


MELSOFT

Engineering Software

MX Sheet Version 3 Operating Manual

-SW3DND-SHEET-E

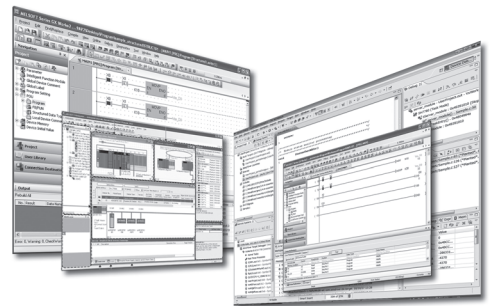

SAFETY PRECAUTIONS

(Read these precautions before using this product.)

Before using this product, please read this manual and the relevant manuals carefully and pay full attention to safety to handle the product correctly. If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.

The precautions given in this manual are concerned with this product. For the safety precautions of the programmable controller system, refer to the user's manual for the module used and MELSEC iQ-R Module Configuration Manual.

In this manual, the safety precautions are classified into two levels: "⚠ WARNING" and "⚠ CAUTION".

WARNING

Indicates that incorrect handling may cause hazardous conditions, resulting in death or severe injury.

CAUTION

Indicates that incorrect handling may cause hazardous conditions, resulting in minor or moderate injury or property damage.

Under some circumstances, failure to observe the precautions given under "⚠ CAUTION" may lead to serious consequences.

Observe the precautions of both levels because they are important for personal and system safety.

Make sure that the end users read this manual and then keep the manual in a safe place for future reference.

[Design Precautions]

WARNING

- When data change, program change, or status control is performed from a personal computer to a running programmable controller, create an interlock circuit outside the programmable controller to ensure that the whole system always operates safely.

Furthermore, for the online operations performed from a personal computer to a CPU module, the corrective actions against a communication error due to such as a cable connection fault should be predetermined as a system.

[Design Precautions]

CAUTION

- The online operations performed from a personal computer to a running CPU module (forced output and operating status changes) must be executed after the manual has been carefully read and the safety has been ensured.

The operation failure may cause the injury or machine damage.

[Security Precautions]

WARNING

- To maintain the security (confidentiality, integrity, and availability) of the programmable controller and the system against unauthorized access, denial-of-service (DoS) attacks, computer viruses, and other cyberattacks from external devices via the network, take appropriate measures such as firewalls, virtual private networks (VPNs), and antivirus solutions.
-

CONDITIONS OF USE FOR THE PRODUCT

- (1) MELSEC programmable controller ("the PRODUCT") shall be used in conditions;
- i) where any problem, fault or failure occurring in the PRODUCT, if any, shall not lead to any major or serious accident; and
 - ii) where the backup and fail-safe function are systematically or automatically provided outside of the PRODUCT for the case of any problem, fault or failure occurring in the PRODUCT.
- (2) The PRODUCT has been designed and manufactured for the purpose of being used in general industries. MITSUBISHI ELECTRIC SHALL HAVE NO RESPONSIBILITY OR LIABILITY (INCLUDING, BUT NOT LIMITED TO ANY AND ALL RESPONSIBILITY OR LIABILITY BASED ON CONTRACT, WARRANTY, TORT, PRODUCT LIABILITY) FOR ANY INJURY OR DEATH TO PERSONS OR LOSS OR DAMAGE TO PROPERTY CAUSED BY the PRODUCT THAT ARE OPERATED OR USED IN APPLICATION NOT INTENDED OR EXCLUDED BY INSTRUCTIONS, PRECAUTIONS, OR WARNING CONTAINED IN MITSUBISHI ELECTRIC USER'S, INSTRUCTION AND/OR SAFETY MANUALS, TECHNICAL BULLETINS AND GUIDELINES FOR the PRODUCT.
- ("Prohibited Application")
- Prohibited Applications include, but not limited to, the use of the PRODUCT in;
- Nuclear Power Plants and any other power plants operated by Power companies, and/or any other cases in which the public could be affected if any problem or fault occurs in the PRODUCT.
 - Railway companies or Public service purposes, and/or any other cases in which establishment of a special quality assurance system is required by the Purchaser or End User.
 - Aircraft or Aerospace, Medical applications, Train equipment, transport equipment such as Elevator and Escalator, Incineration and Fuel devices, Vehicles, Manned transportation, Equipment for Recreation and Amusement, and Safety devices, handling of Nuclear or Hazardous Materials or Chemicals, Mining and Drilling, and/or other applications where there is a significant risk of injury to the public or property.
- Notwithstanding the above restrictions, Mitsubishi Electric may in its sole discretion, authorize use of the PRODUCT in one or more of the Prohibited Applications, provided that the usage of the PRODUCT is limited only for the specific applications agreed to by Mitsubishi Electric and provided further that no special quality assurance or fail-safe, redundant or other safety features which exceed the general specifications of the PRODUCTS are required. For details, please contact the Mitsubishi Electric representative in your region.
- (3) Mitsubishi Electric shall have no responsibility or liability for any problems involving programmable controller trouble and system trouble caused by DoS attacks, unauthorized access, computer viruses, and other cyberattacks.

INTRODUCTION

Thank you for purchasing the engineering software, MELSOFT series.

This manual is designed for users to understand operations of MX Sheet.

Before using the product, thoroughly read this manual and related manuals to develop full familiarity with the functions and performance of MX Sheet and supported modules to ensure correct use.

Note that the menu names and operating procedures may differ depending on an operating system in use and its version.

When reading this manual, replace the names and procedures with the applicable ones as necessary.

CONTENTS

SAFETY PRECAUTIONS	1
CONDITIONS OF USE FOR THE PRODUCT	2
INTRODUCTION	3
RELEVANT MANUALS	7
GENERIC TERMS AND ABBREVIATIONS	7
CHAPTER 1 FUNDAMENTALS OF MX Sheet	8
1.1 Before Using This Product	8
Using MX Sheet	9
Operating considerations	12
1.2 Main Functions of MX Sheet	17
Logging function	17
Monitor function	17
Write function	17
Automatic save function	18
Automatic print function	18
Create Button function	18
1.3 System Configuration	19
System configuration	19
Accessible range	19
Operating environment	20
1.4 Screen Configuration and Basic Operations	22
Operation procedure for MX Sheet	22
MX Sheet menu	25
Basic operations of MX Sheet	27
Logical station number	43
CHAPTER 2 FUNCTION LIST OF MX Sheet	44
CHAPTER 3 CELL SETTING	46
3.1 Operation of "Cell Settings" Screen	46
3.2 When "Logging" is Selected	47
Setting of the [Use] tab	48
Setting of the [Access Data] tab	55
Setting of the [Operation Interval] tab	61
Setting of the [Device Trigger] tab	67
Setting of the [Handshake] tab	69
Setting of the [CSV Logging] tab	80
3.3 When "Monitor" is Selected	83
Setting of the [Use] tab	84
Setting of the [Access Data] tab	87
Setting of the [Operation Interval] tab	88
Setting of the [Device Trigger] tab	89
Setting of the [Handshake] tab	90
Setting of the [CSV Logging] tab	91
3.4 When "Write" is Selected	92
Setting of the [Use] tab	93
Setting of the [Access Data] tab	95

Setting of the [Operation Interval] tab	97
Setting of the [Device Trigger] tab	98
Setting of the [Handshake] tab	99
3.5 When "Alarm Summary" is Selected	100
Setting of the [Use] tab	101
Setting of the [Access Data] tab	104
Setting of the [Alarm Data] tab	106
Setting of the [Operation Interval] tab	108
Setting of the [Device Trigger] tab	109
3.6 When "Comment" is Selected	110
Setting of the [Use] tab	111
Setting of the [Access Data] tab	112
Setting of the [Comment Data] tab	114
Setting of the [Operation Interval] tab	116
Setting of the [Device Trigger] tab	117
Setting of the [Handshake] tab	118
CHAPTER 4 AUTOMATIC SAVE SETTING	119
<hr/>	
4.1 Operation of "Automatic Save List" Screen	119
4.2 Setting of "Automatic Save" Screen	120
CHAPTER 5 AUTOMATIC PRINT SETTING	126
<hr/>	
5.1 Operation of "Automatic Print List" screen	126
5.2 Setting of "Automatic Print" Screen	127
CHAPTER 6 AUTOMATIC COMMUNICATION STARTUP/CANCELLATION	129
<hr/>	
6.1 "Automatic Communication Startup"	129
6.2 Cancelling "Automatic Communication Startup"	129
CHAPTER 7 START COMMUNICATION AND END COMMUNICATION	131
<hr/>	
7.1 Start Communication	131
7.2 End Communication	133
CHAPTER 8 1 SHOT COMMUNICATION	134
<hr/>	
CHAPTER 9 EDITING CELLS	136
<hr/>	
9.1 Cutting Cell Area	136
9.2 Copying Cell Area	137
9.3 Pasting Cell Area	138
9.4 Deleting Cell Area	140
CHAPTER 10 CHANGING SHEET NAME	141
<hr/>	
CHAPTER 11 CREATING BUTTONS	143
<hr/>	
11.1 Start Communication Button	143
11.2 End Communication Button	147
11.3 1 Shot Communication Button	148
CHAPTER 12 PROTECTING/UNPROTECTING MX Sheet SETTING	149
<hr/>	
12.1 Protecting MX Sheet Setting	149

12.2	Unprotecting MX Sheet Setting	151
CHAPTER 13 OPTIONS		152
13.1	Setting Error Logs	152
	"ErrorLog" sheet	153
13.2	Protecting a workbook	155
CHAPTER 14 EXPORTING SETTING DATA		156
CHAPTER 15 SAMPLE PROGRAMS		158
APPENDIX		160
Appendix 1 Additions and Changes from Previous Version		160
Appendix 2 Processing Speed of MX Sheet		161
	Performance values	161
	Number of processable device points when using system labels	162
Appendix 3 Processing MX Sheet		163
	Collection delay and data dropout	163
	Logging function	167
Appendix 4 Creating the Excel Spreadsheet for MX Sheet		169
	Communication efficiency and cell area specifying method	169
	Communication efficiency and access data setting	170
	Communication efficiency and use of Excel function (cell reference)	171
Appendix 5 Procedure to Transport Data to Other Personal Computer		173
Appendix 6 HTML File		174
	HTML file	174
	Convenient use of HTML file	174
Appendix 7 CSP+ For Machine		175
Appendix 8 Warning Messages on Windows		176
Appendix 9 Troubleshooting		177
	Considerations for deleting a temporary file	178
	Countermeasures for errors as a result of setting the automatic communication startup setting in an Excel book and opening it in Microsoft Excel 2007 or later	179
	Countermeasures when MX Sheet add-ins remain in the EXCEL add-in list	182
Appendix 10 Useful Functions		183
	Alarm summary	183
	Comment display	183
	Device trigger	184
	Handshake	185
	CSV logging	186
	Automatic communication startup	186
	Protecting MX Sheet setting	186
	Setting error logs	187
Appendix 11 Compatibility With Existing Products		188
REVISIONS		189
INFORMATION AND SERVICES		190
TRADEMARKS		190
COPYRIGHTS		190

RELEVANT MANUALS

Manual name [manual number]	Description	Available form
MX Sheet Version 3 Operating Manual [SH-082390ENG] (this manual)	Operation procedures, setting and operation methods of MX Sheet	e-Manual PDF
MX Component Version 5 Reference Manual [SH-082395ENG]	Operation method, programming procedures, and error codes of MX Component Version 5	e-Manual PDF

Point

e-Manual refers to the Mitsubishi Electric FA electronic book manuals that can be browsed using a dedicated tool.

e-Manual has the following features:

- Required information can be cross-searched in multiple manuals.
- Other manuals can be accessed from the links in the manual.
- Hardware specifications of each part can be found from the product figures.
- Pages that users often browse can be bookmarked.

GENERIC TERMS AND ABBREVIATIONS

Unless otherwise specified, this manual uses the following generic terms and abbreviations.

Generic term/abbreviation	Description
Ethernet communication	Communication by connecting a personal computer to an Ethernet module or a built-in Ethernet CPU.
Ethernet Built-in CPU	A CPU module with an Ethernet port
FXCPU	FX3SCPU, FX3GCPU, FX3GCCPU, FX3UCPU, FX3UCCPU
GOT	Mitsubishi Electric Graphic Operation Terminal GOT1000 series, GOT2000 series
Q motion CPU	Q172DCPU, Q173DCPU, Q172DSCPU, Q173DSCPU
R Motion CPU	R16MTCPU, R32MTCPU
Inverter	FREQROL-A800 series
Robot controller	CR750-D/CRnD-700 series

1 FUNDAMENTALS OF MX Sheet

1.1 Before Using This Product

MX Sheet is a communication support software package that allows device data collection, etc. by simple, programless setting using Excel®.

Logging function

Monitor function

Automatic print function

Alarm summary function

Write function

Comment display function


Automatic save function

Excel book file
HTML file
CSV file

Error log setting function

Protect MX Sheet setting function

Create button function

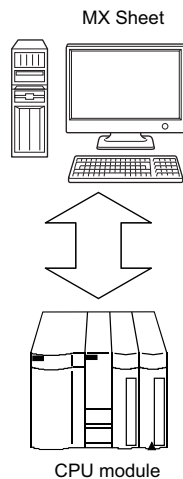


Using MX Sheet


Program-less and easy setting

Device data of a CPU module can be collected/written by simple setting without programming.

MX Sheet

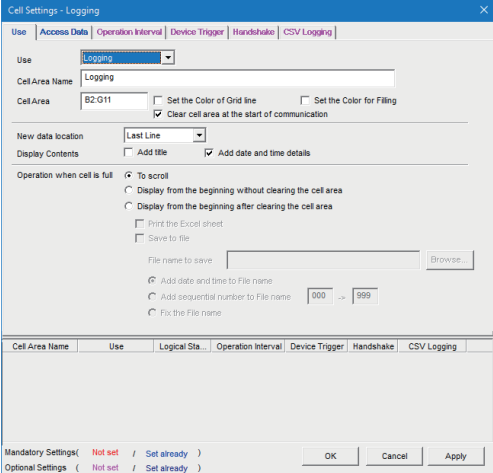

Excel

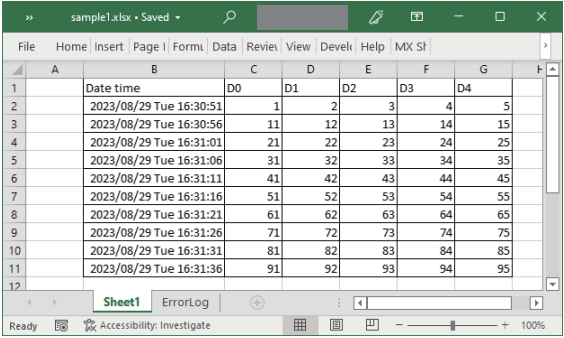

➔ Performing simple setting ➔

CPU module device data is displayed on Excel spreadsheet.


Collecting/writing device data using a wide range of communication routes

MX Sheet uses MX Component for communication between a CPU module and personal computer.


Using a variety of communication routes supported by MX Component, system configuration that meets user's requirement can be achieved.

Examples of communication using MX Component


- Ethernet communication

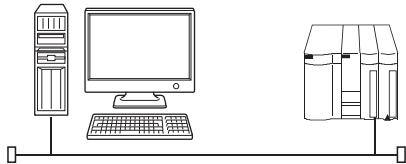

- MELSECNET/H communication

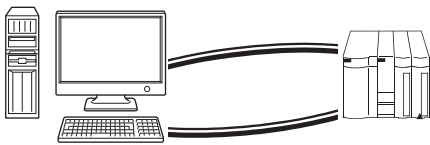

- GOT Gateway Device communication

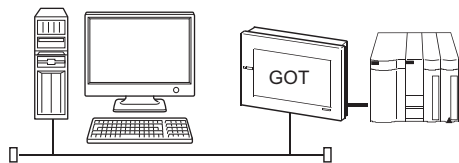


Displaying and setting data with labels

Not only devices, but also the data with labels can be displayed/set.

Register the labels by using Label Utility of MX Component.

Using the system labels controlled by MELSOFT Navigator enables sharing labels with the iQ Works supported products.

There are two types of system labels for MELSOFT Navigator: system label ver.1 and system label ver.2.

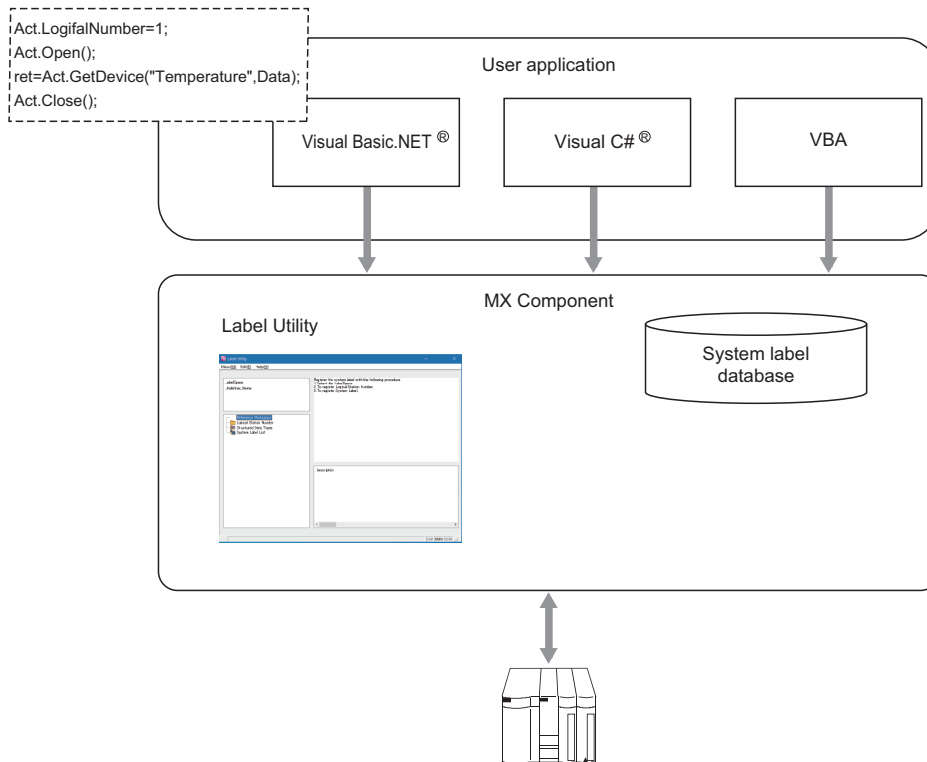


Controlling each function by device condition

Conditions for collecting and writing device data can be set to a device in a CPU module.

The execution of each MX Sheet function can be controlled from the CPU module side.

- When the device data is collected/written while bit device is ON

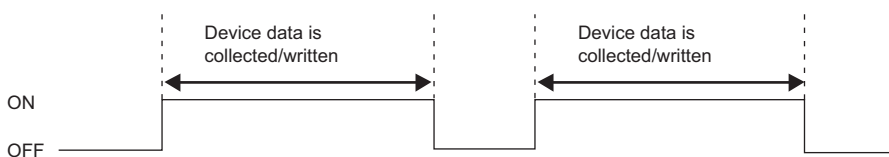


■Corresponding functions

- Logging
- Monitor
- Write
- Alarm summary
- Comment display
- Automatic save
- Automatic print

Data logging using CSV file

Using the logging or monitor function, device data can be displayed on Excel spreadsheet, and collected data can be saved into a CSV file simultaneously.

Long-term data collection is available with a single CSV file.

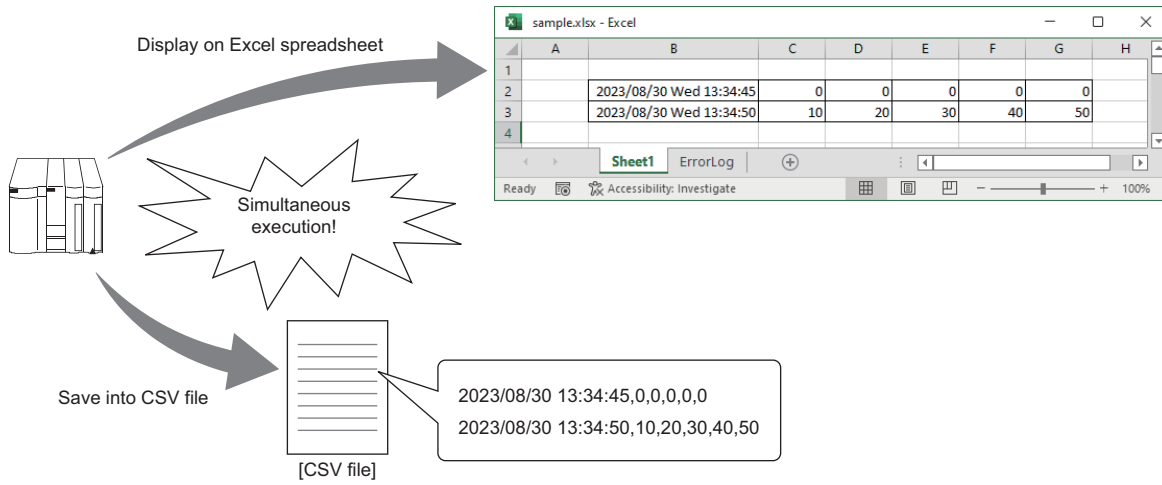

Operating considerations

This section explains the considerations in the following order.

- Considerations of operating system and personal computer to be used
- Considerations for setting MX Sheet
- Considerations for setting cells and Excel spreadsheets
- Considerations for performing communication
- Considerations for using VBA
- Considerations for using other MELSOFT products

Considerations of operating system and personal computer to be used

■Administrator authority when setting/changing communication setup

A user with the administrator authority must log on to set or change Communication Settings.

■Coexistence of different Excel versions

When different versions of Excel exist in a single personal computer, MX Sheet does not operate normally.

■Resume function, etc. of personal computer

If any of the following is set to a personal computer where MX Sheet is installed, a communication error occurs during communication with a CPU module.

Do not set any of the following functions on the personal computer.

- Resume function
- Suspend function
- Power saving function
- Standby mode

Considerations for setting MX Sheet

■Word designation for bit and bit designation for word

In the following tabs and screens, word designation for bit (e.g. K4M0) and bit designation for word (e.g. D0.0) cannot be set.

- [Access Data] tab (Digit-specified bit device (e.g. D0.0) can be set.)
- [Device Trigger] tab
- [Handshake] tab
- "Automatic Save" screen
- "Automatic Print" screen

■Reading character strings

When character strings are read from the CPU module, the device data which prefix is either of the following characters are not displayed properly on an Excel spreadsheet.

When reading character strings from the CPU module, set proper setting so that either of the following characters are not prefixed.

- = (equal)
- ' (single quotation)

■Saving Excel spreadsheets

MX Sheet saves Excel book at the timing of closing the "Cell Settings" screen. Before editing data, backing up the Excel book is recommended.

If the file name specified in the "Automatic Save" screen or "Operating when cell is full" of the [Use] tab already exists, the old data is discarded and overwritten.

Therefore, make sure that the specified file name is different from other Excel book names.

■Excel file location

Choose a local folder as the file location for an Excel file to be used in MX Sheet. If the file is synchronized with OneDrive, etc., disable the synchronization.

■Operation when opening multiple Excel books

- Do not operate other Excel book during the operation of a settings screen of MX Sheet.
- When selecting the [Arrange All] menu in the [View] tab in Excel, the display of selectable menu items in the [MX Sheet] tab may be changed. (The items may be displayed in the same manner as other Excel books.) Activate the Excel book to display the items correctly.

■Reinstalling Excel

Do not reinstall Excel if MX Sheet has already been installed.

To reinstall Excel, uninstall MX Sheet first.

■Setting COM add-ins

The following COM add-ins are used in MX Sheet.

- MX Sheet Ribbon Add-in
- MX Sheet Add-in

The COM add-ins above can be enabled or disabled from the [COM Add-ins] menu in the [Developer] tab in Excel.

Restart Excel when changing COM add-in settings for MX Sheet in the "COM Add-Ins" screen of Excel.

Note that some add-ins (except for MX Sheet add-ins) may cause MX Sheet not to run properly.

In such case, disable the add-ins.


■Color designation from Excel

If the border color and cell fill color are specified in "Format Cells" in Excel, colors specified in "Set the Color of Grid line" and "Set the Color for Filling" in the [Use] tab become invalid.

■Excel spreadsheet where buttons are placed

When the Start Communication, End Communication or 1 Shot Communication button placed on the Excel spreadsheet is focused, do not log off or exit from Windows without closing the Excel book.

Otherwise, the following message appears, and Excel cannot be closed.

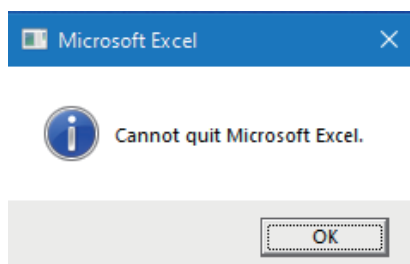

■Setting to handle a large amount of data

The amount of data that can be handled on Excel depends on memory available on a personal computer. When setting to handle a large amount of data on MX Sheet, pay attention to the memory utilization.

■Size of saved Excel file according to the setting of cell formats

On Excel, setting the cell format increases the saved file size.

Also on MX Sheet, the size of the saved Excel file may become several M bytes or more since the cell format is changed according to the setting.

Ex.

Settings that increases the saved file size

- When "Set the Color of Grid line" or "Set the Color for Filling" is selected on the [Use] tab
- When Logging is selected and "Add date and time details" is selected on the [Use] tab
- When "Alarm summary" is selected on the [Use] tab
- When "Character string" is specified as the Data Type on the [Access Data] tab
- When "HEX" is specified as the Value on the [Access Data] tab

Considerations for setting cells and Excel spreadsheets

■ Save function

If either of the following settings is set to an Excel book where the ActiveX controls and forms are applied, it will cause insufficient memory when operating a personal computer continuously.

If insufficient memory occurs, shut down the personal computer periodically.

- Save function of MX Sheet (automatic save function or save is performed when cell is full)
- Save function is called in a VBA program.

It may take time to save the book.

■ Changing Excel spreadsheet name

When changing the sheet name of an Excel spreadsheet where MX Sheet is set, change it from the [MX Sheet] tab ⇔ [Tools] ⇔ [Change Sheet Name].

If the sheet name is changed directly from Excel or from a VBA program, MX Sheet is not operate normally.

If this happens due to sheet name change, set the previous sheet name again.

■ Setting sheet protection of "ErrorLog" sheet

Do not set "Protect Sheet" to an "ErrorLog" sheet.

Otherwise, the "ErrorLog" sheet does not operate properly.

■ "ErrorLog" sheet name

In an Excel book where MX Sheet is set, do not use the name "ErrorLog" to newly created worksheet, chart or dialog sheet.

Otherwise, the "ErrorLog" sheet created by MX Sheet does not operate properly.

Considerations for performing communication

■ Continuous operation of Excel

Excel is not an application that is designed for continuous operation.

For operating MX Sheet continuously, exit and reactivate Excel periodically.

The time for allowable continuous operation differs according to the operating environment.

■ Communication between personal computer and CPU module

When CPU module device data is collected/written using MX Sheet, the communication restrictions that apply to MX Component also occur between a personal computer and CPU module.

For the restrictions on communications between the personal computer and CPU module, refer to the following:

 MX Component Version 5 Reference Manual

■ Preview setting of Excel

When starting the communication of MX Sheet, do not activate the preview setting (print preview, etc.) of Excel.

If the communication of MX Sheet is started with the preview setting of Excel active, a memory leak occurs.

■ Simultaneous communication from multiple Excel books

Multiple Excel books where MX Sheet setting is set cannot be started on a single personal computer to perform communication simultaneously.

■ Double-starting Excel books

Excel books with the same name can not be double-started.

■ When logoff/shutdown is executed during communication

Do not log off or shut down a personal computer during usual communication or 1 shot communication.

Log off or shut down the personal computer after terminating the communication with a CPU module and exiting from Excel.

■USB communication

A communication error may occur and it may not be recovered if connecting and disconnecting a USB cable, resetting a CPU module, or turning the power ON or OFF is performed frequently during communication with the CPU module.

If the operation is not recovered from an error, remove the USB cable. Then, connect it again after five or more seconds. (Even after this operation, an error may occur at initial communication. However, communication will be successful after that.)

■Operation of Excel during communication


● If Excel is in either of the following status, MX Sheet cannot execute operations on Excel (e.g. displaying data into cells, saving or printing an Excel book).

- A cell is in input status (e.g. a cell is double-clicked, or the cursor is at the formula bar).
- A message or a dialog box is displayed on Excel.

● The operation of Excel during communication is restricted as follows.


- Tabs on the ribbon are hidden.

Although tabs except for the [MX Sheet] tab (such as the [File] tab, etc.) and the quick access toolbar are displayed, do not operate them during communication.

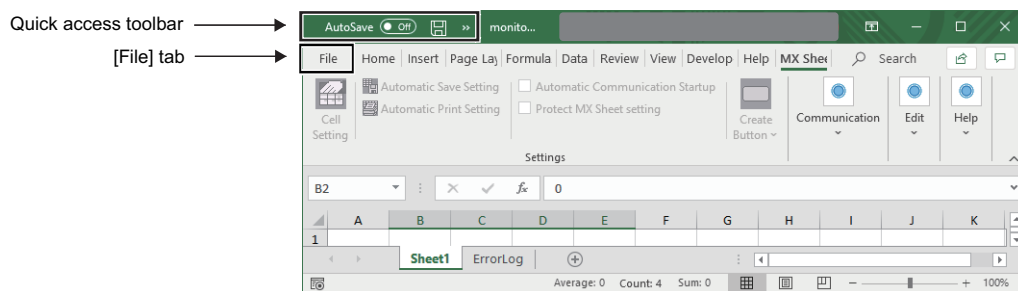


■Mouse cursor during communication

While MX Sheet is communicating, the mouse cursor setting of an Excel spreadsheet is fixed to "Normal Select" in "Mouse Properties".

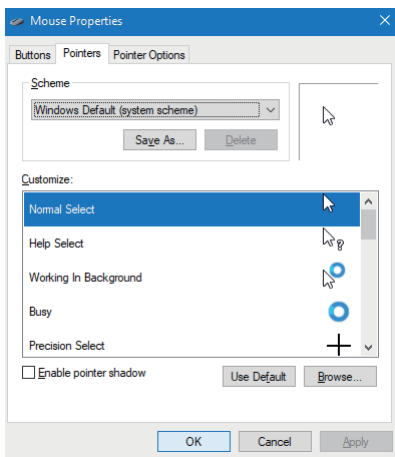

■Change to Design Mode of Excel during communication

For Excel during communication, do not change to Design Mode. Otherwise, MX Sheet may not operate properly.

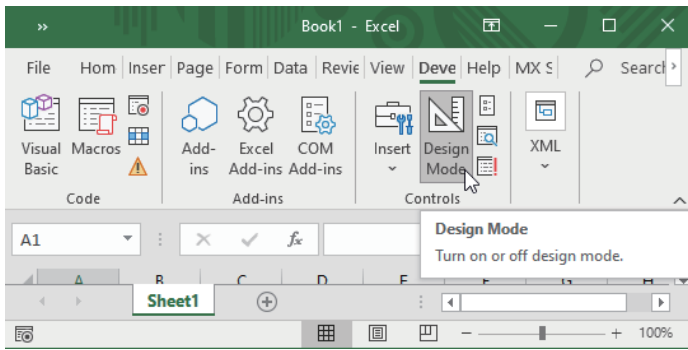

Considerations for using VBA

■Incorporation of VBA program

When incorporating a user-created VBA program into an Excel spreadsheet where MX Sheet is set, check the operation of the VBA program before creating programming in the Excel spreadsheet.

If the user-created VBA program is executed during communication of MX Sheet, the communication processing of MX Sheet may be interrupted with an error message of Excel displayed. By closing the error message, the communication processing resumes.

■VBA program creation

MX Sheet utilizes OLE Automation for communication.

Do not perform the following on VBA programs.

- Do not execute the DoEvents method in a For-Next loop.
- FileFilter is ignored in the GetSaveAsFileName method.
- Do not execute the Reset method in the Excel menu.

Considerations for using other MELSOFT products

■Version of MX Component

When using MX Sheet, MX Component Version 5 or later is required.

■Logical station number


Before deleting a logical station number (➤ Page 43 Logical station number) from Communication Settings Utility of MX Component, check that the logical station number to be deleted is not used in MX Sheet.

If the logical station number used in MX Sheet is deleted, MX Sheet does not operate normally.

1.2 Main Functions of MX Sheet

Logging function



Accumulates device data collected from a programmable controller as history in the cell area selected on an Excel spreadsheet. (Page 27 Logging)

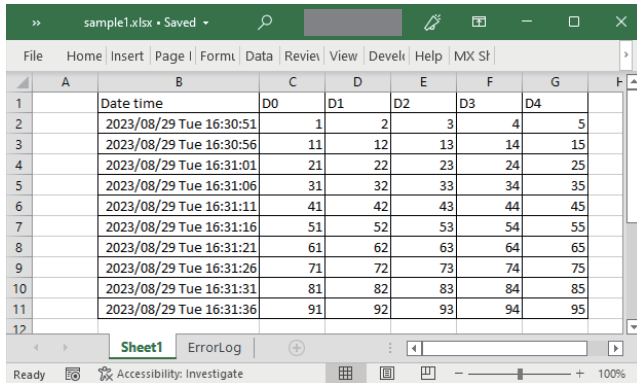

Device data is accumulated as history.

Monitor function

Displays device data collected from a programmable controller in the cell area selected on an Excel spreadsheet. (Page 33 Monitoring)


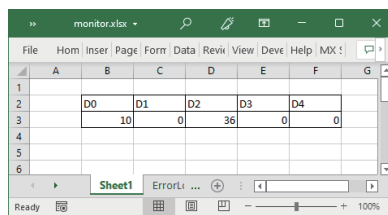


CPU module

Programmable controller data is displayed on Excel.

Write function

Writes values entered on an Excel spreadsheet to a programmable controller device. (Page 35 Writing data)

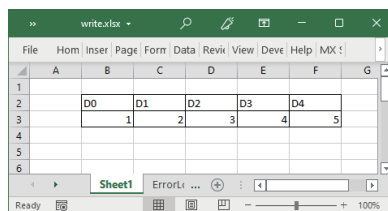

CPU module

Values entered on Excel are written to programmable controller devices.

Automatic save function

Automatically saves an Excel book. (☞ Page 37 Automatic saving)

Automatic save is performed in the time specification and device trigger.

Automatic print function

Automatically prints an Excel book or a specified Excel spreadsheet. (☞ Page 40 Automatic printing)

Automatic printing is performed in the time specification and device trigger.

Create Button function

Executes the Start Communication, End Communication, and 1 Shot Communication functions by merely clicking the corresponding button. (☞ Page 42 Creating/Using button)


1.3 System Configuration

The system configuration for MX Sheet is the same as that for MX Component Version 5.
 For details, refer to the following:

MX Component Version 5 Reference Manual

System configuration

In this manual, the following system configuration is used to explain an example of operation.

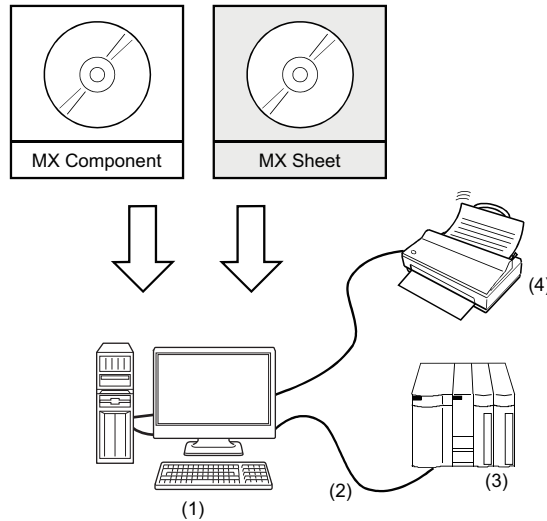

No.	Item	Description	
(1)	Personal computer	Personal computers that meet the operation environment of MX Sheet MX Sheet Version 3 Installation Instructions	
	Software	OS	Microsoft® Windows 10 Pro Operating System (English version)
		MX Sheet	MX Sheet Version 3
		MX Component	MX Component Version 5
		Excel	Microsoft Excel for Microsoft 365 (64-bit version) (English)
(2)	USB cable	MR-J3USBCBL3M	
(3)	CPU module	R16CPU	
(4)	Printer	Printers that support the specification of the personal computer	

Accessible range

Accessible CPUs

The accessible CPUs in MX Sheet are the same as those in MX Component Version 5.

For details, refer to the following:

MX Component Version 5 Reference Manual

Accessible device ranges

The accessible device ranges in MX Sheet are the same as those in MX Component Version 5, except for the following item.

For details, refer to the following:

MX Component Version 5 Reference Manual

■ Device extension representation

MX Sheet does not allow access to any device by word designation for bit device (e.g. K4X0, K8M0) and bit designation for word device (e.g. D0.0, W0.1).

Specifying GOT timer contact devices and counter contact devices

In the cell settings of MX Sheet (☞ Page 46 CELL SETTING), timer contact devices (TT) and counter contact devices (CT) which are the device representation of GOT can be entered.

The entered "TT" and "CT" are automatically changed to "TS" and "CS" respectively.

Specifying devices on Q motion CPU

The device write function cannot be executed.

Device indexing (bit specification, digit specification, indexed addressing) cannot be used.

Operating environment

Item	Description	
Personal computer	A personal computer on which Microsoft Windows operates	
CPU	Windows 11	2 or more cores on a compatible 64-bit processor or System on a Chip (SoC)
	Windows 10	Processor 1.6 GHz with 2 or more cores
Required memory	Windows 11	4 GB or more recommended
	Windows 10	2 GB or more recommended
Available hard disk capacity	<ul style="list-style-type: none"> For installation: 2.5 GB or more free hard disk capacity^{*1} For operation: 512 MB or more free virtual memory capacity 	
Monitor	Windows 11	Resolution WXGA (1280 × 720 pixels) or higher
	Windows 10	Resolution 1024 × 768 pixels or higher
OS (English version) (32-bit version/64-bit version)	<ul style="list-style-type: none"> Windows 11 (Home, Pro, Enterprise, Education)^{*2} Windows 10 (Home, Pro, Enterprise, Education, IoT Enterprise 2016 LTSC^{*2}, IoT Enterprise 2019 LTSC^{*2}) 	
Required software (English version)	<ul style="list-style-type: none"> Microsoft Excel 2019 (32-bit version/64-bit version)^{*3}, Microsoft Excel 2021 (32-bit version/64-bit version)^{*3*4}, Microsoft Excel for Microsoft 365 (64-bit version)^{*5} MX Component Version 5 	

*1 Includes free space required for installing MX Component.

*2 64-bit version only

*3 Desktop version only

*4 The operation of this product has been confirmed with the version 2206 (Build 15330.20196).

*5 The operation of this product has been confirmed with the version 2201 (Build 14827.20192).

.NET Framework 4.6 Advanced Services and .NET Framework 4.8 Advanced Services need to be enabled. For details, refer to TECHNICAL BULLETIN No. FA-A-0207.

This product may not operate properly when using any of the following functions:

- Application start-up in Windows compatibility mode
- Fast user switching
- Remote desktop
- Touch function
- Virtual environment such as Client Hyper-V
- Tablet mode
- Virtual Desktops
- Windows hibernate or standby
- Unified Write Filter
- Text cursor indicator

In the following cases, the screen of this product may not work properly.

- The size of the text and other items in the screen is other than 100% (96 DPI, 9 pt etc.).
- The resolution of the screen is changed in operation.
- The Windows theme is changed in operation.
- The multi-display is set.

Excel spreadsheets created in the English environment are applicable to the English environment only, cannot be used in the other environment.

In this product, the period (.) is used as the symbol of the decimal point. Regardless of the setting of "Decimal symbol" on the control panel, use the period when entering the decimal point.

Precautions

- A communication error may occur when communicating with a CPU module after setting the resume function, suspend setting, power-saving function, and/or standby mode of a personal computer.
Therefore, when communicating with the CPU module, do not set the above functions.
- Surrogate pair characters and environment dependent characters are not available in MX Sheet.

1.4 Screen Configuration and Basic Operations

Operation procedure for MX Sheet

Operating procedure

1. Set the security setting of Excel. (☞ Page 22 Security settings of Excel)
2. Check if MX Sheet is installed properly. (☞ Page 24 Checking if the installation is completed properly)
3. Start Excel and save an Excel book.*1
4. Select the function to be used (☞ Page 25 MX Sheet menu), and set the MX Sheet setting. (☞ Page 27 Basic operations of MX Sheet)
5. Start the communication. (☞ Page 131 Start Communication)
6. End the communication. (☞ Page 133 End Communication)

*1 Save an Excel file to be used in MX Sheet to a local folder. If the file is synchronized with OneDrive, etc., disable the synchronization.





Communication efficiency differs depending on the MX Sheet setting. (☞ Page 161 Processing Speed of MX Sheet, ☞ Page 169 Creating the Excel Spreadsheet for MX Sheet)

Security settings of Excel


The following explains the security setting procedure that is required for using MX Sheet.

Operating procedure

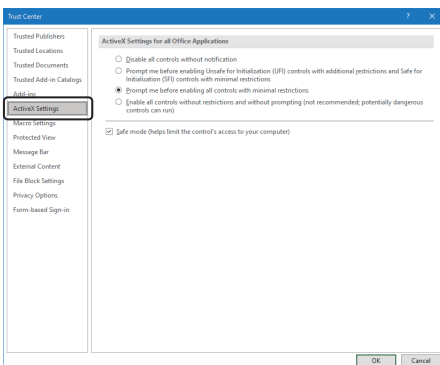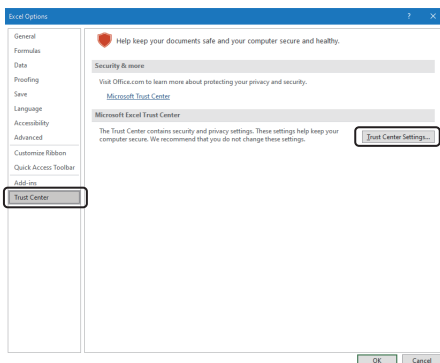

1. Select [File] ⇒ [Options] in Excel, and open the "Excel Options" screen. Select "Trust Center" from the list on the left side of the screen, and click the [Trust Center Settings] button.

2. Select "ActiveX Settings" from the list on the left side of the screen, and select the items other than "Disable all controls without notification."

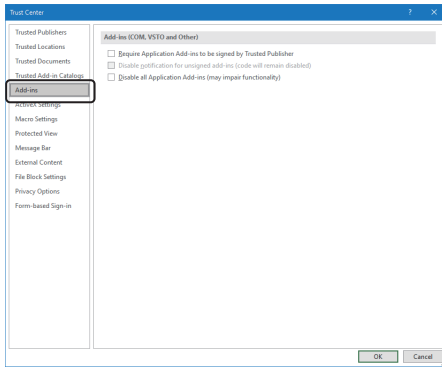


3. Select "Add-ins" from the list on the left side of the screen, and unselect all the checkboxes.

Checking if the installation is completed properly

The following explains a procedure for checking if the installation of MX Sheet is completed normally.


1. Start Excel.

If the following screens appear, click the [Install] button.

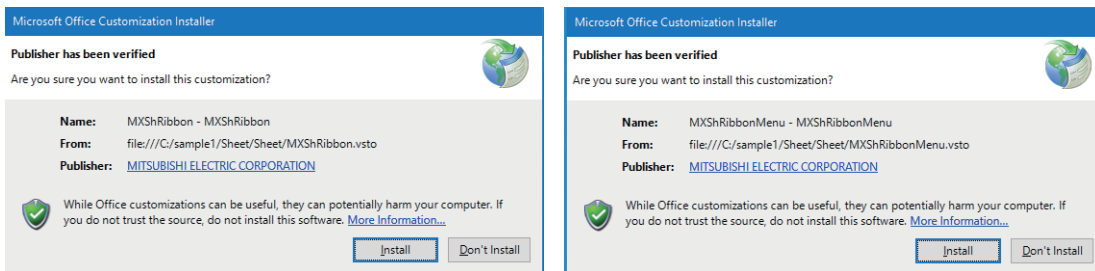

2. Check that the following items are selected in the "COM Add-Ins" screen.

- MX Sheet Ribbon Add-in
- MX Sheet Add-in

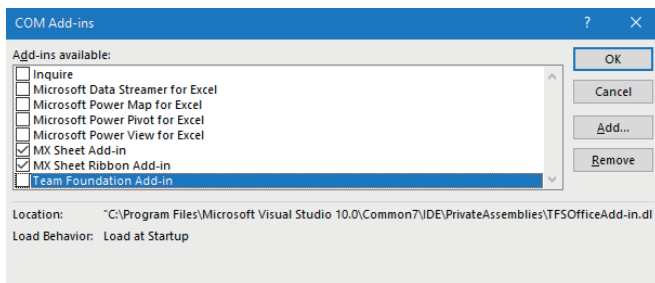

3. Check that the [MX Sheet] tab is added, and the menu bar, icons, and groups of MX Sheet (☞ Page 26 Menu, icons, and groups) are added.

Administrator authority when setting/changing communication setup

Administrator authority is required for setting/changing communication setup.

Operating procedure

Select Communication Settings Utility, and then right-click and select [Run as administrator].

MX Sheet menu

The following explains a procedure for displaying the menu to select a function of MX Sheet and details on the items to be selected.

Operating procedure















- Select the [MX Sheet] tab.
- Specify the cell area and right-click.

Point

If the Excel spreadsheet type is other than a worksheet, the MX Sheet menu is not displayed.
When using MX Sheet, set the setting on a worksheet.

Details of MX Sheet menu

The following table shows the details of each MX Sheet menu item.

Item			Description	Reference	
Group ^{*1}	Menu ^{*1}	Icon ^{*1}			
Setting	Cell Setting ^{*2}		Set the cell setting.	Page 46 CELL SETTING	
	Automatic Save Setting		Set the automatic save setting.	Page 119 AUTOMATIC SAVE SETTING	
	Automatic Print Setting		Set the automatic print setting.	Page 126 AUTOMATIC PRINT SETTING	
	Automatic Communication Startup	—	Start or cancel automatic communication.	Page 129 AUTOMATIC COMMUNICATION STARTUP/ CANCELLATION	
	Protect MX Sheet setting	—	Protect or unprotect the MX Sheet setting.	Page 149 PROTECTING/ UNPROTECTING MX Sheet SETTING	
	Create Button	—		Select the "Create Button" menu.	Page 143 CREATING BUTTONS
		Start Communication Button	—	Create the start communication button.	Page 143 Start Communication Button
End Communication Button		—	Create the end communication button.	Page 147 End Communication Button	
1Shot Communication Button		—	Create the 1 shot communication button.	Page 148 1 Shot Communication Button	
Communication	Start		Start communication.	Page 131 Start Communication	
	End ^{*3}		End communication.	Page 133 End Communication	
	1Shot ^{*2}		Perform 1 shot communication.	Page 134 1 SHOT COMMUNICATION	
Edit	Cell Area	—		Select the "Cell Area" menu.	Page 136 EDITING CELLS
		Cut Cell Area ^{*2}		Cut a cell area.	Page 136 Cutting Cell Area
		Copy Cell Area ^{*2}		Copy a cell area.	Page 137 Copying Cell Area
		Paste Cell Area ^{*2*4}		Paste a cell area.	Page 138 Pasting Cell Area
		Delete Cell Area ^{*2}		Delete a cell area.	Page 140 Deleting Cell Area
	Tools	—		Select the "Tools" menu.	Page 152 OPTIONS
		Change Sheet Name		Change the Excel spreadsheet name.	Page 141 CHANGING SHEET NAME
		Setting Data Export	—	Export settings.	Page 156 EXPORTING SETTING DATA
		Options	—	Set options for communication.	Page 152 Setting Error Logs

Item			Description	Reference
Group *1	Menu *1	Icon *1		
Help	Help	—	Start e-Manual Viewer and display the manual.	Page 42 Displaying the manual
	Version Info.	—	Display the MX Sheet version.	Page 42 Confirming method of MX Sheet version

*1 Displayed on the ribbon after selecting the [MX Sheet] tab. (Page 26 Menu, icons, and groups)


*2 Can also be selected from the menu displayed by specifying a cell area and right-clicking it.

*3 Can be selected after start of communication.

*4 Can be selected after the cell area is cut or copied.

■Menu, icons, and groups

These are displayed on the ribbon after selecting the [MX Sheet] tab.

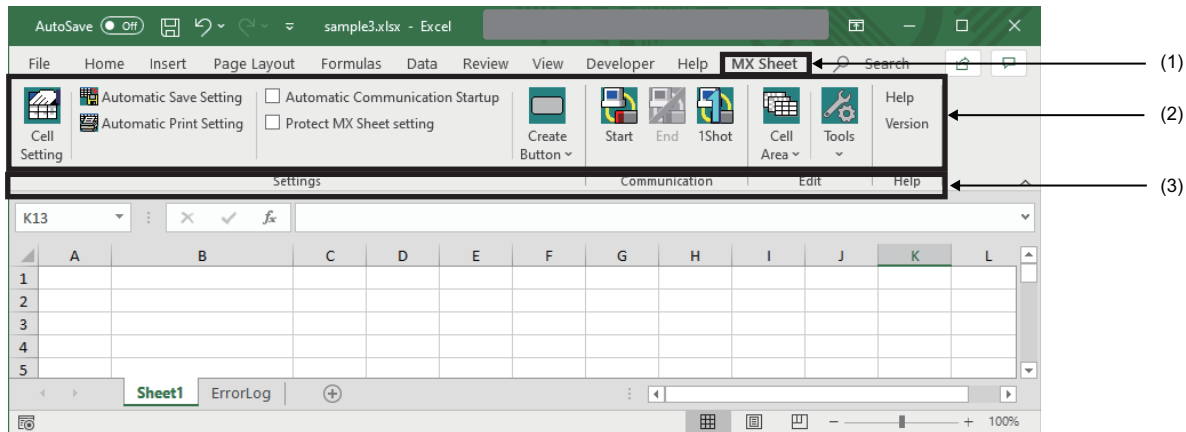

(1) [MX Sheet] tab

(2) Menu (items) and icons (images)


(3) Groups

Basic operations of MX Sheet

Logging


The following explains an example of creating an Excel spreadsheet using the logging function.

Window



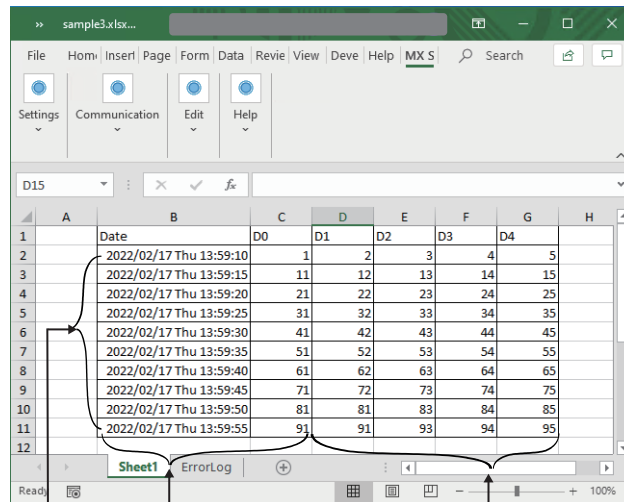


- Logging times are displayed. Contents of D0 to D4 are displayed in order from left to right.
- 10 units of logging data are displayed.
 - The latest logging data is displayed on the last line.
 - Scrolled up in order.

Operating procedure

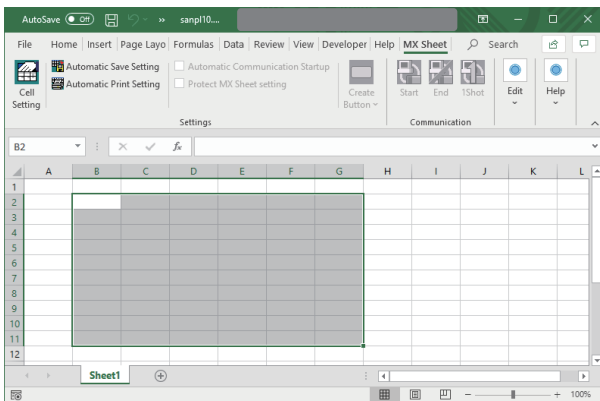

1. Start Excel and select [File] ⇒ [Save As] to save an Excel book with a new name.
2. Drag the cells (B2 to G11 in this example) on the left screen to specify the cell area in which logging data is to be displayed.

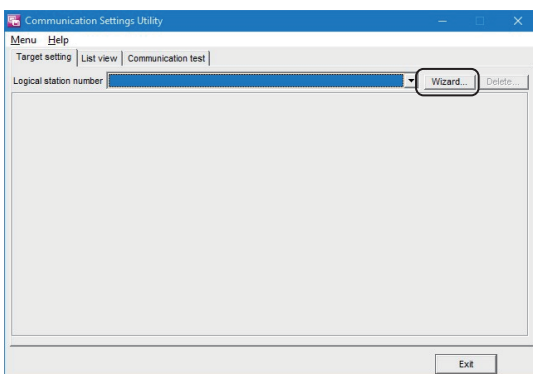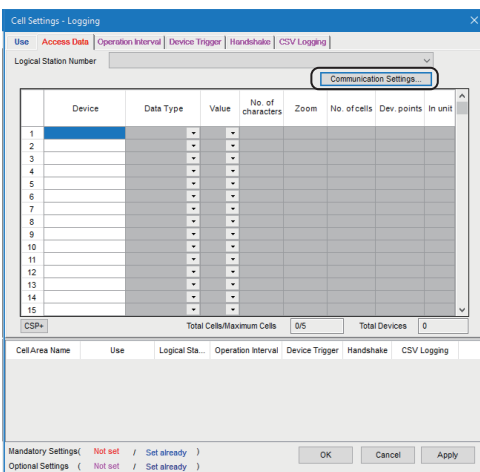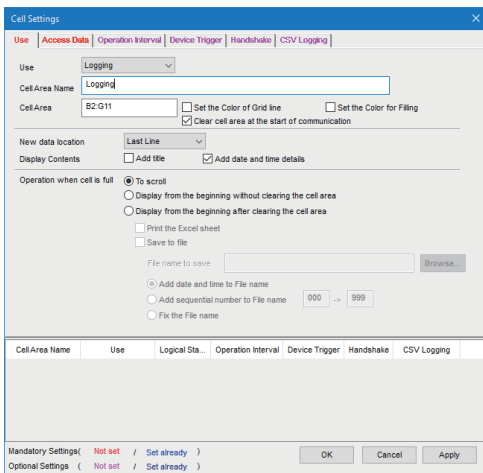


3. Select the [MX Sheet] tab ⇒ [Cell Setting] to display the "Cell Settings" screen.

Set the following items of the [Use] tab.

- Use: Logging
- Cell Area Name: Logging
- Cell Area: B2:G11
- New data location: Last Line
- Display Contents: Add date and time details
- Operation when cell is full: To scroll




After completing the settings, select the [Access Data] tab.

4. Click the [Communication Settings] button to start Communication Settings Utility for setting a logical station number (Page 43 Logical station number). When the following screen appears, click the [Yes] button.

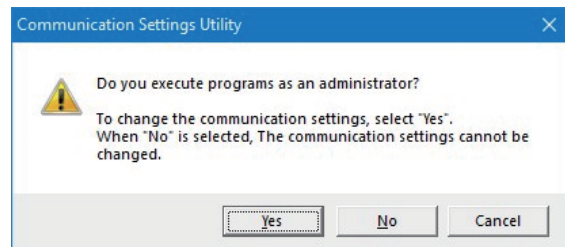

The "User Account Control" screen appears. Click the [Yes] button.

5. After starting Communication Settings Utility, select the [Target setting] tab and click the [Wizard] button.

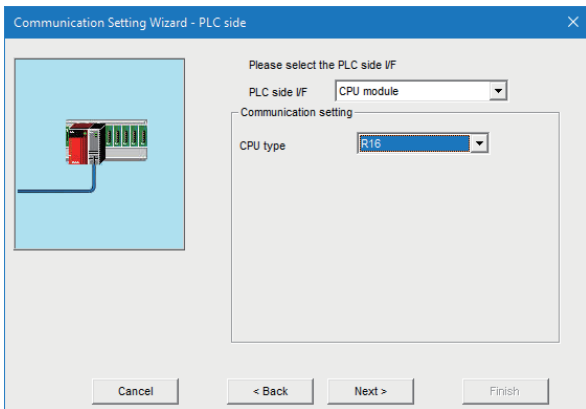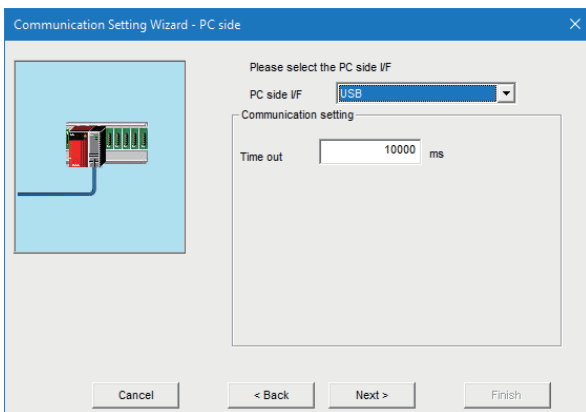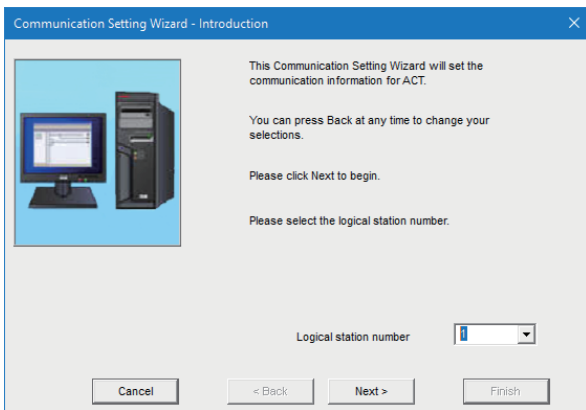





6. Set "1" in "Logical station number" and click the [Next] button.

7. Set the personal computer side interface as follows, and click the [Next] button.

- PC side I/F: USB
- Time out: 10000

8. Set the programmable controller side interface as follows, and click the [Next] button.

- PLC side I/F: CPU module
- CPU type: R16

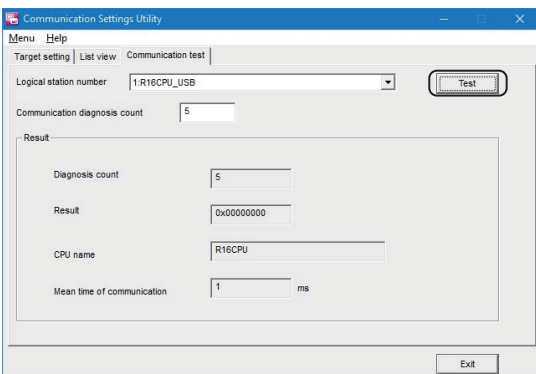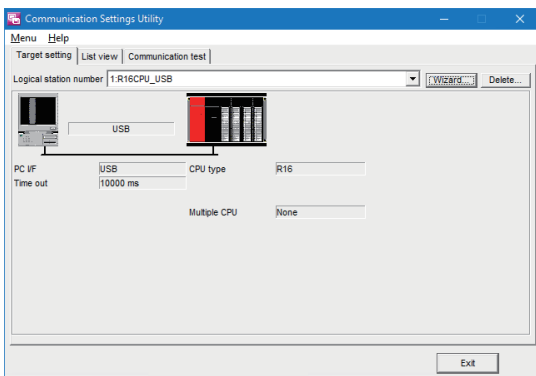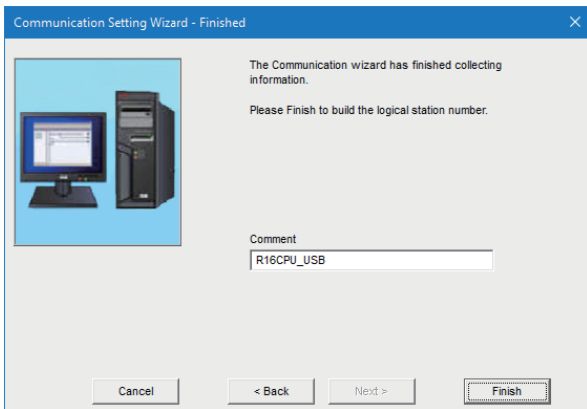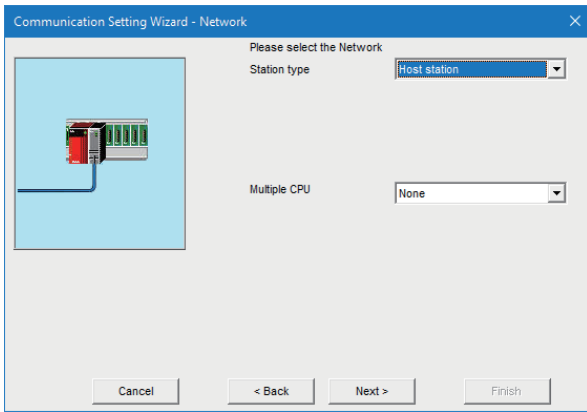

9. Select the communication route as follows, and click the [Next] button.

- Station type: Host station
- Multiple CPU: None

10. Enter any word (R16CPU_USB in this example) and click the [Finish] button.

11. Check if the logical station number settings displayed on the [Target setting] tab of Communication Settings Utility are correct.

After checking, select the [Communication test] tab.

12. Click the [Test] button to check that the programmable controller and personal computer are normally communicating.

After confirmation, click the [Exit] button to close Communication Settings Utility.

An error message appears if they are not communicating normally.

Check the error definition and remove the error.

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	D0	16bit integer	DEC		1	5	5	Word
2								
3								
4								
5								
6								
7								
8								
9								
10								
11								
12								
13								
14								
15								

Total Cells/Maximum Cells: 5/5
Total Devices: 5



Set the Operation Interval

Operation day: Daily Weekly Monthly

Operation time: Regular interval (5 s) Minutely Hourly Time table

Logging Time zone: Log Always Log only during the specified time zone



CellArea Name: Logging
Use: Logging
Logical Sta.: 1.R16CPU_...
Operation Interval: Settings
Device Trigger: No settings
Handshake: No settings
CSV Logging: No settings



13. Set the device to be logged as follows on the [Access Data] tab.

- Logical Station Number: 1
- Device: D0
- Data Type: 16bit integer
- Value: DEC
- Zoom: 1
- No. of cells: 5

Labels can be set to "Device."

When a system label is set to "Device," "1" is displayed to "No. of cells" and cannot be changed.


After completing the settings, select the [Operation Interval] tab.

14. Set the logging operation interval as follows.


- Set the Operation Interval: Selected
- Operation day: Daily
- Operation time: Regular interval (5 seconds)
- Logging Time zone: Log Always

15. Click the [Apply] button to enable the settings of the "Cell Settings" screen.



Check that the cell area is registered in the screen shown on the left, and click the [OK] button.

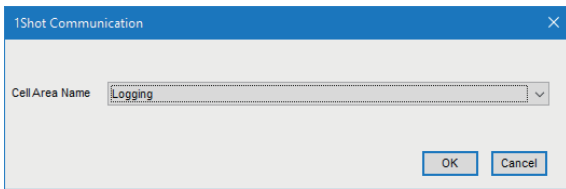

• Before adjustment

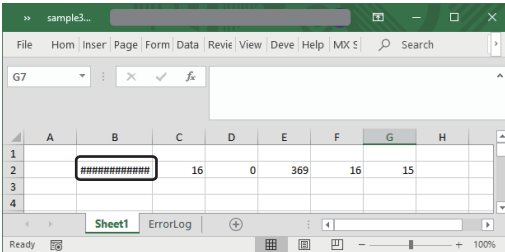

• After adjustment

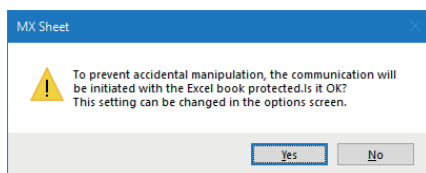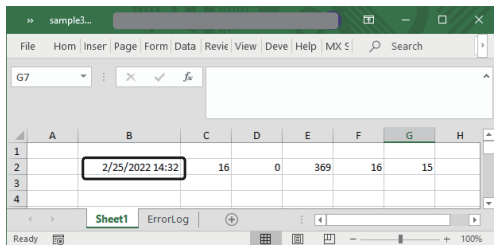

16. Check if the settings from step 1 to 15 are correct by using the 1 shot communication function of MX Sheet.

Perform 1 shot communication in the following procedure.

- 1** Select the [MX Sheet] tab ⇒ [1Shot].
- 2** Select the cell area name set in step 3 ("Logging function" in this example) for "Cell Area Name" in the "1Shot Communication" screen.
- 3** Click the [OK] button to start 1 shot communication.

17. After 1 shot communication, "#####" is displayed in the date/time cell as shown on the left screen.

Adjust the cell width of Column B so that the date and time can be displayed.

18. Select the [MX Sheet] tab ⇒ [Start].

Click the [Yes] button in the displayed message, and start logging.


The displayed message differs depending on option settings and the workbook protection status. (Page 145 Property setting)

19. Select the [MX Sheet] tab ⇒ [End] to end logging.

Monitoring

The following explains an example of creating an Excel spreadsheet using the monitor function.



Window

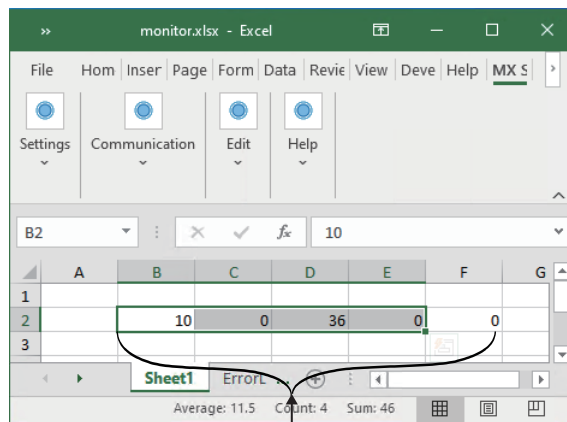




Access data D0 to D4 are displayed in order from left to right.

Operating procedure

1. Start Excel and select [File] ⇒ [Save As] to save an Excel book with a new name.
2. Drag the cell (B2 to F2 in this example) on the left screen to specify the cell area in which monitor data is displayed.

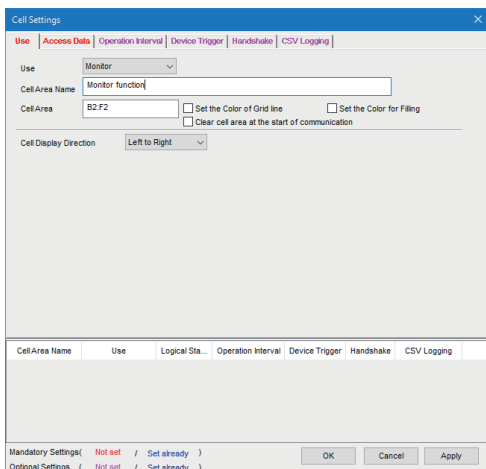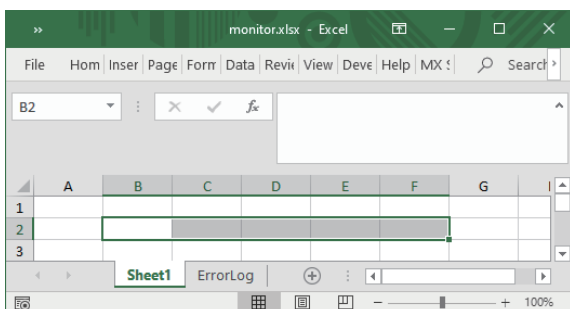

3. Select the [MX Sheet] tab ⇒ [Cell Setting] to display the "Cell Settings" screen.
Set the following items of the [Use] tab.
- Use: Monitor
 - Cell Area Name: Monitor function
 - Cell Area: B2:F2
 - Cell Display Direction: Left to Right
- After completing the settings, select the [Access Data] tab.

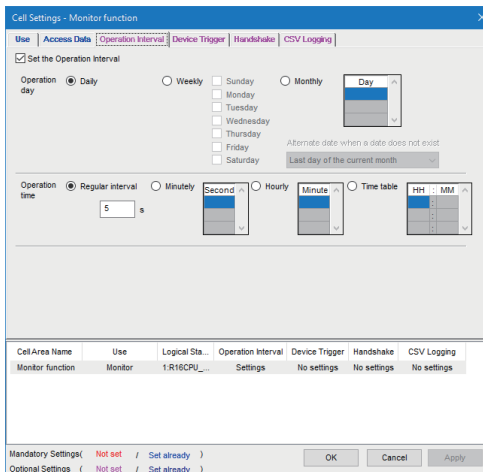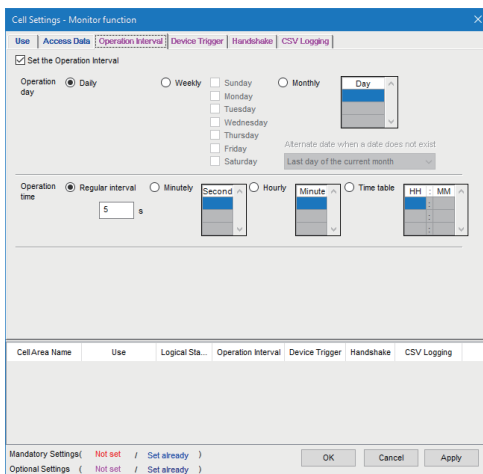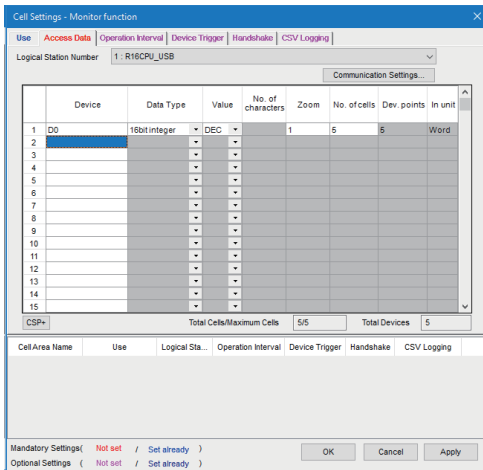

4. Set the device to be monitored as follows.

- Logical Station Number: 1
- Device: D0
- Data Type: 16bit integer
- Value: DEC
- Zoom: 1
- No. of cells: 5

For the logical station number setting method, refer to the following:

Page 43 Logical station number

Labels can be set to "Device."

When a system label is set to "Device," "1" is displayed to "No. of cells" and cannot be changed.


After completing the settings, select the [Operation Interval] tab.

5. Set the monitor operation interval as follows.

- Set the Operation Interval: Selected
- Operation day: Daily
- Operation time: Regular interval (5 seconds)

6. Click the [Apply] button to enable the settings of the "Cell Settings" screen.

Check that the cell area is registered in the screen shown on the left, and click the [OK] button.

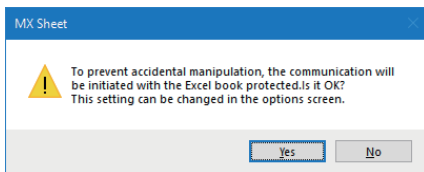


7. Check if the settings from step 1 to 6 are correct by using the 1 shot communication function of MX Sheet. Perform 1 shot communication in the following procedure.
 - ① Select the [MX Sheet] tab ⇒ [1Shot].
 - ② Select the cell area name set in step 3 ("Monitor function" in this example) for "Cell Area Name" in the "1Shot Communication" screen.
 - ③ Click the [OK] button to start 1 shot communication.
8. Select the [MX Sheet] tab ⇒ [Start]. Click the [Yes] button in the displayed message, and start monitoring. The displayed message differs depending on option settings and the workbook protection status. (Page 145 Property setting)
9. Select the [MX Sheet] tab ⇒ [End] to exit monitor. After ending the communication, delete the monitor data.

Writing data


The following explains an example of creating an Excel spreadsheet using the write function.

Window



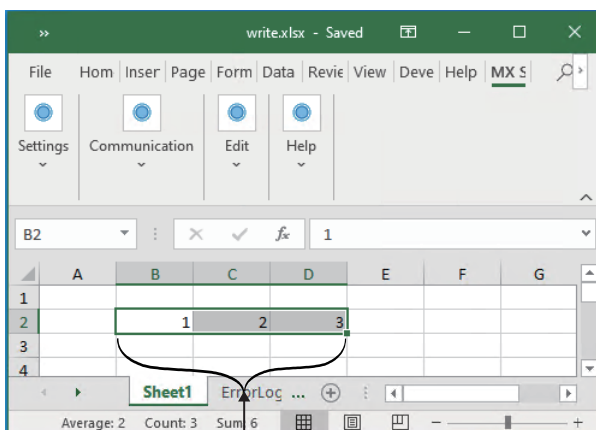


Enter values to be written to D0 - D2 in order from left to right.

Operating procedure

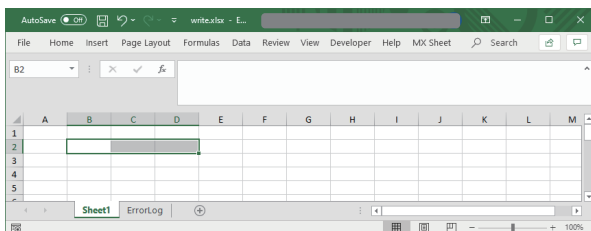

1. Start Excel and select [File] ⇒ [Save As] to save an Excel book with a new name.
2. Drag the cell (B2 to D2 in this example) on the left screen to specify the cell area in which monitor data is displayed.

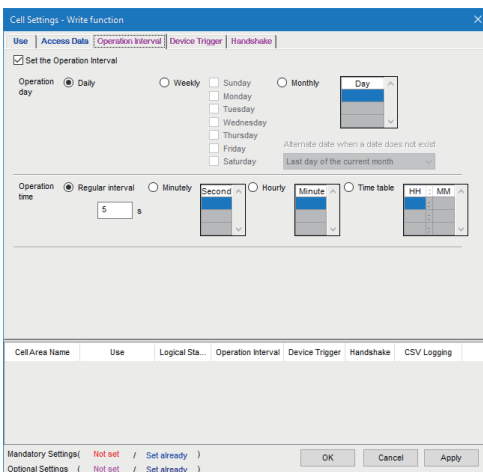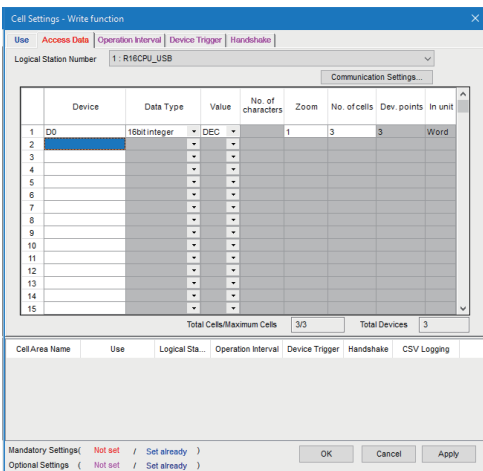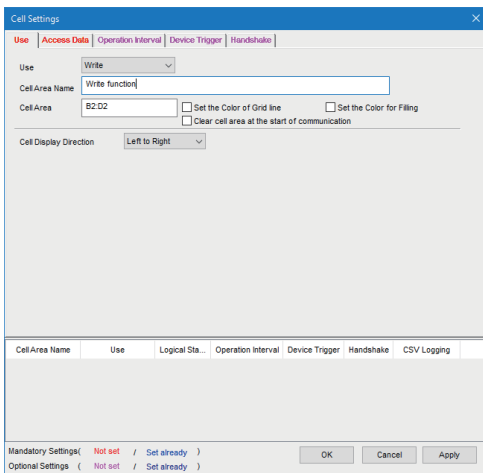

3. Select the [MX Sheet] tab ⇒ [Cell Setting] to display the "Cell Settings" screen.

Set the following items of the [Use] tab.

- Use: Write
- Cell Area Name: Write function
- Cell Area: B2:D2
- Cell Display Direction: Left to Right

After completing the settings, select the [Access Data] tab.

4. Set the device to be written as follows.

- Logical Station Number: 1
- Device: D0
- Data Type: 16bit integer
- Value: DEC
- Zoom: 1
- No. of cells: 3

For the logical station number setting method, refer to the following:

Page 43 Logical station number




Labels can be set to "Device."

When a system label is set to "Device," "1" is displayed to "No. of cells" and cannot be changed.

After completing the settings, select the [Operation Interval] tab.

5. Set the writing operation interval as follows.

- Set the Operation Interval: Selected
- Operation day: Daily
- Operation time: Regular interval (5 seconds)

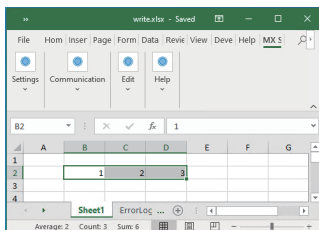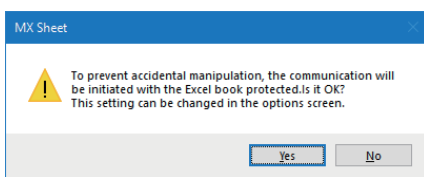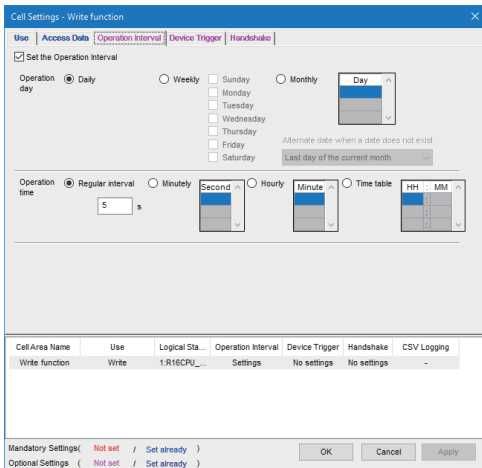

6. Click the [Apply] button to enable the settings of the "Cell Settings" screen.

Check that the cell area is registered in the screen shown on the left, and click the [OK] button.

7. Select the [MX Sheet] tab ⇒ [Start].

Click the [Yes] button in the displayed message, and start writing data.

The displayed message differs depending on option settings and the workbook protection status. (Page 145 Property setting)

8. Enter the values to be written to devices into the cell area specified in step 2.

- Cell B2: 1 (value to be written to D0)
- Cell C2: 2 (value to be written to D1)
- Cell D2: 3 (value to be written to D2)

Check that the data on Excel are written to the programmable controller devices.


9. Select the [MX Sheet] tab ⇒ [End] to end writing.

Automatic saving

The following explains a procedure for saving an Excel book during MX Sheet operation automatically.

- Automatic save condition: Save when the device (Y0) turns on.
- Automatically saved file name: Add date and time to the file name of auto.xlsx.



Window

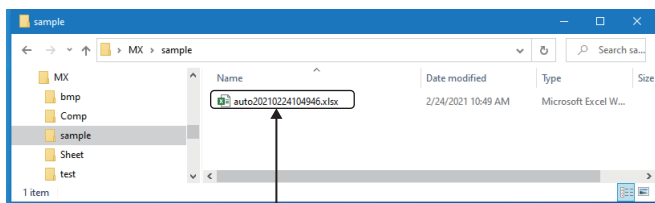

Automatically saved Excel file

Operating procedure

1. Start Excel and select the [MX Sheet] tab ⇒ [Automatic Save Setting] to display the "Automatic Save List" screen.
2. Click the [Create New] button to create new automatic save conditions.

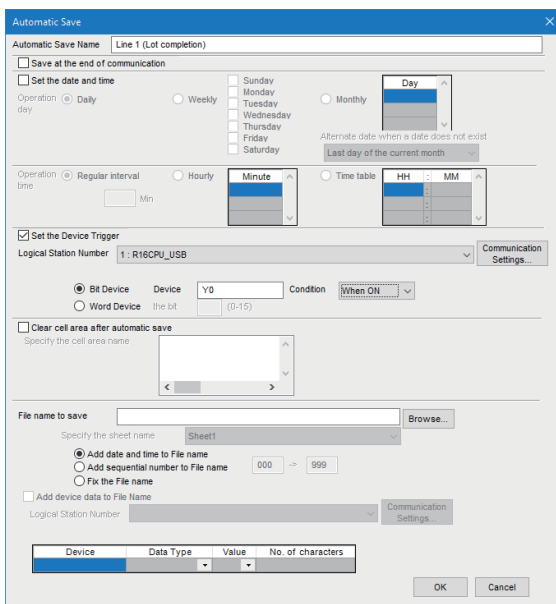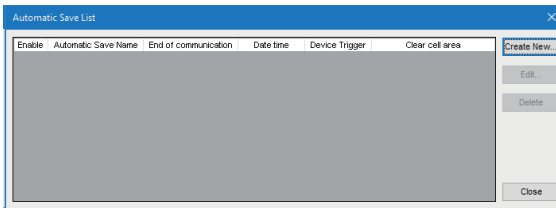

3. Set the automatic save conditions as follows.
 - Automatic Save Name: Line 1 (Lot completion)
 - Set the Device Trigger: Selected
 - Logical Station Number: 1
 - Bit Device: Selected
 - Device: Y0
 - Condition: When ON
 - Add date and time to File name: Selected

For the logical station number setting method, refer to the following:

Page 43 Logical station number

Labels can be set to "Device."

Set the file name to be saved automatically.



Clicking the [Browse] button displays the "Save As" screen.

Specify any save place and file name.

- File name: auto.xlsx
- Save as type: Excel Workbook (*.xlsx)




After specifying the file name, click the [Save] button.

After completing the above settings, click the [OK] button.

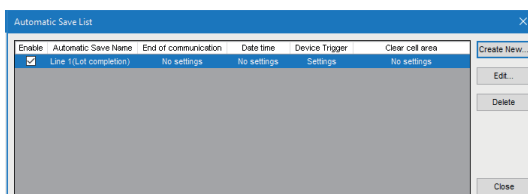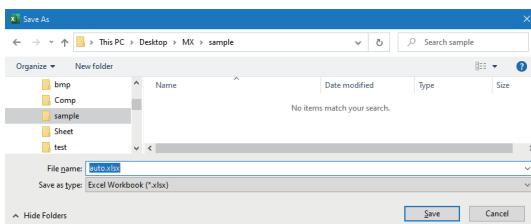

4. The automatic save name is added to the list. Check that the check box of "Enable" is selected, click the [Close] button to close the "Automatic Save List" screen.



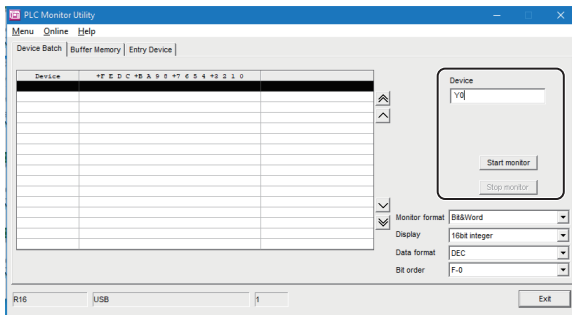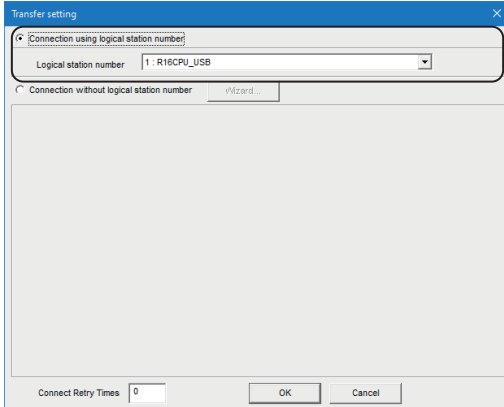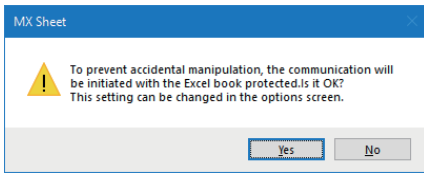

5. Select the [MX Sheet] tab ⇒ [Start].

Click the [Yes] button in the displayed message, and start the communication.

The displayed message differs depending on option settings and the workbook protection status. (☞ Page 145 Property setting)

6. Start PLC controller monitor utility.

As the "Transfer setting" screen is displayed, set the following items.


- Connection using logical station number: Selected
- Logical station number: 1

After completing the above settings, click the [OK] button.

7. Select the [Device Batch] tab of the "PLC Monitor Utility" screen and set the following items.

- Device: Y0

After completing the settings, click the [Start monitor] button.

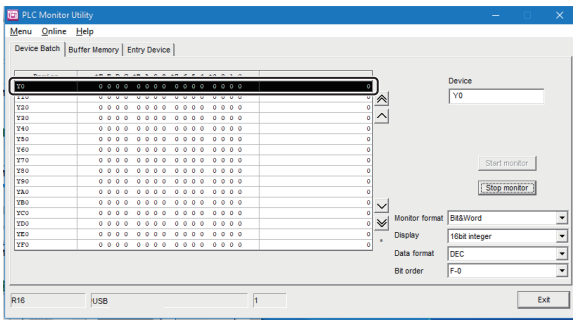

8. Change the Y0 device status.



Double-click the monitor display area of the [Device Batch] tab to display the "Write to Device" screen.

Forcibly turn ON Y0 in the following procedure.

❶ Enter "Y0" in "Device" in "Bit device."


❷ Click the [Force ON] button.

After completing the above settings, click the [Close] button.

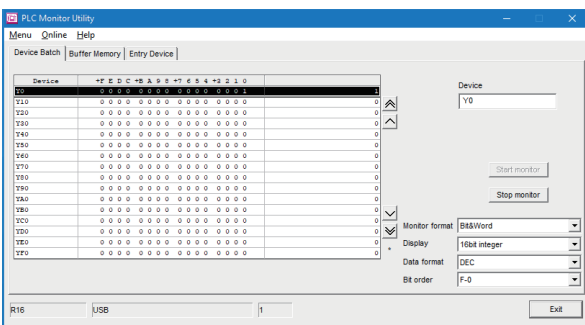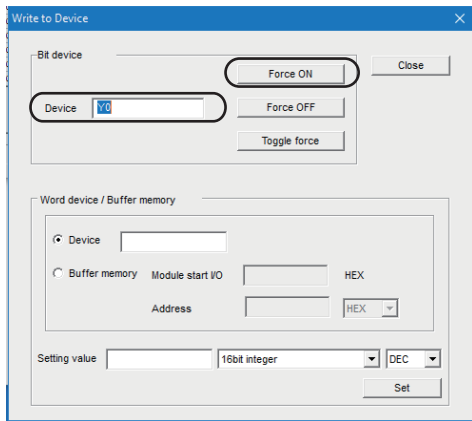

9. Check that Y0 is turned ON as set in step 8.

After checking, click the [Stop monitor] button and then the [Exit] button.

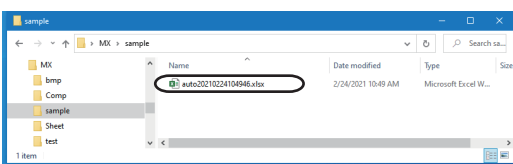

10. The operation in step 8 activates the automatic save setting function, and saves the Excel book automatically.

Start Explorer and check if the file specified in step 3 is saved correctly.

After checking the file, select the [MX Sheet] tab ⇒ [End] to end communication.

Automatic printing




The following explains a setting procedure for automatically printing the whole Excel book or specified Excel spreadsheets during the MX Sheet operation.

- Automatic print condition: Printed at 17:00 every day.
- Print area: Sheet 1 and Sheet 3 are printed.

Operating procedure

1

1. Start Excel and select the [MX Sheet] tab ⇒ [Automatic Print Setting] to display the "Automatic Print List" screen.
2. Click the [Create New] button to create new automatic print conditions.

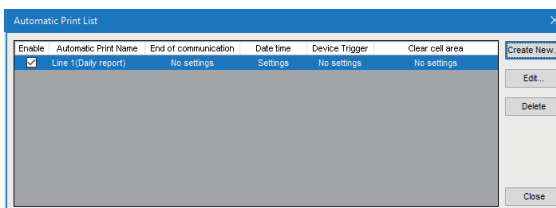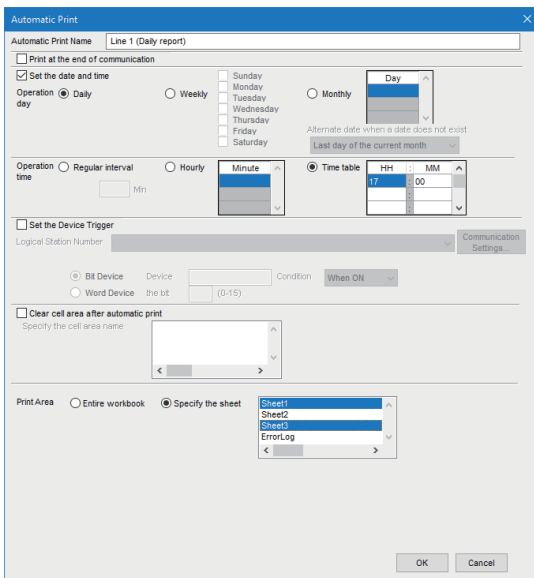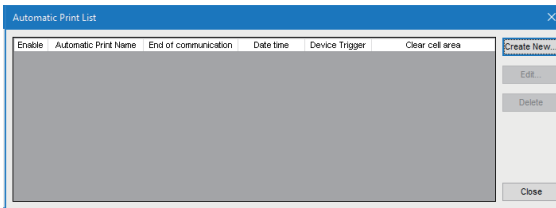


3. Set the automatic print conditions as follows.
 - Automatic Print Name: Line 1 (Daily report)
 - Set the date and time: Selected
 - Operation day: Daily
 - Operation time: Time table (17:00)
 - Print Area: Specify the sheet (Sheet 1 and Sheet 3)Multiple spreadsheets can be selected. After the settings, click the [OK] button.


4. The automatic print name is added to the list. Check that the check box of "Enable" is selected, click the [Close] button to close the "Automatic Print List" screen.

Creating/Using button

The following explains a convenient communication starting method by Create Button.

- Button type: Start Communication button
- MX Sheet setting condition: Logging setting ( Page 27 Logging)


Operating procedure

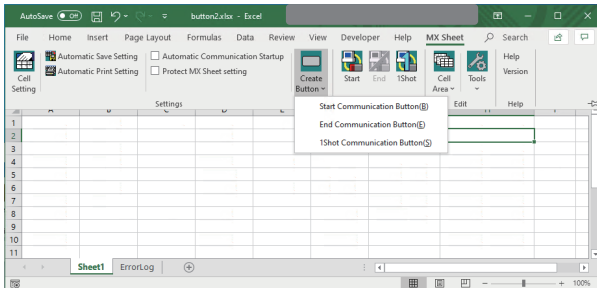


1. Start Excel and specify the cell where the button is placed.


Select the [MX Sheet] tab ⇒ [Create Button] ⇒ [Start Communication Button].


The start communication button is placed in the specified cell position.

The display characters on the created button can be changed. ( Page 145 Property setting)

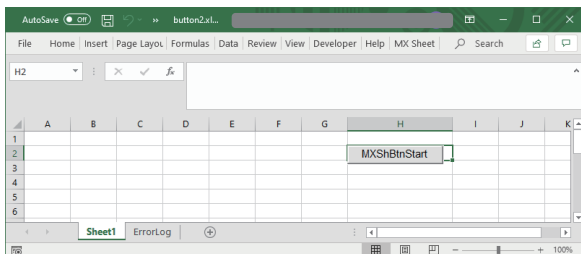

2. Click the start communication button created in step 1. Click the [Yes] button in the displayed message.

The displayed message differs depending on option settings and the workbook protection status. ( Page 145 Property setting)

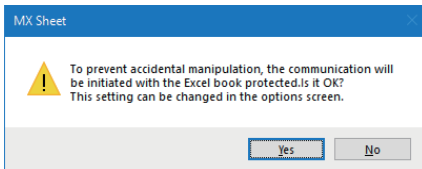

Displaying the manual

Help is used for checking the operation method.

Window

[MX Sheet] tab ⇒ [Help]

e-Manual Viewer starts and the manual appears.

Confirming method of MX Sheet version

This section explains how to confirm the MX Sheet version.

Confirm the MX Sheet version in the "Product information about MX Sheet" screen.


Window

[MX Sheet] tab ⇒ [Version]

Logical station number

The logical station number is the logical number assigned to the data that is the compilation of the connection-destination information necessary to open a communication line into a single data by Communication Settings Utility.

In MX Sheet, communication is performed by using the logical station number set by Communication Settings Utility of MX Component.

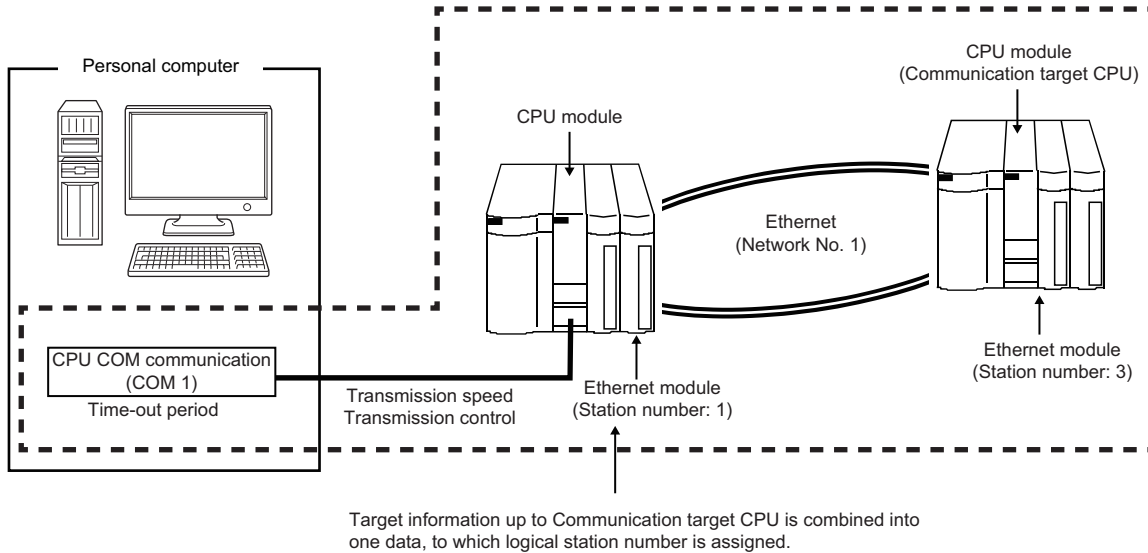

2 FUNCTION LIST OF MX Sheet

Function Name	Description	Available device points	Available cells	Reference
Logging	Accumulates device data collected from a CPU module as history in the cell area selected on Excel.	256 points ^{*1*2}	256 columns × 1000000 rows	Page 47 When "Logging" is Selected
Monitor	Displays device data collected from a CPU module in the cell area selected on Excel.	2000 points ^{*1*3}	2000	Page 83 When "Monitor" is Selected
Write	Writes values entered on Excel to a CPU module.	2000 points ^{*1*3}	2000	Page 92 When "Write" is Selected
Alarm summary	Converts ON/OFF data of bit devices into alarm comment character strings that are set separately and accumulates them on Excel spreadsheet as alarm history.	2000 points ^{*2*4}	6 columns × 65536 rows	Page 100 When "Alarm Summary" is Selected
Comment display	Converts bit or word device values into comment character strings that are set separately and displays them on Excel spreadsheet.	1 point ^{*5}	1	Page 110 When "Comment" is Selected
Device trigger	Collects/Writes device data when set device conditions set for collection/write are met.	—	—	Page 67 Setting of the [Device Trigger] tab
Handshake	Sets handshake with a CPU module for secure device data collection/write.	—	—	Page 69 Setting of the [Handshake] tab
CSV logging	Displays device data on Excel spreadsheet with logging or monitor function, and simultaneously saves collected data as a CSV file.	—	—	Page 91 Setting of the [CSV Logging] tab
Automatic save	Automatically saves Excel book.	—	—	Page 119 AUTOMATIC SAVE SETTING
Automatic print	Automatically prints Excel book.	—	—	Page 126 AUTOMATIC PRINT SETTING
Automatic communication startup	Automatically starts communication with a CPU module when Excel book is started.	—	—	Page 129 AUTOMATIC COMMUNICATION STARTUP/CANCELLATION
Start communication	Starts communication with a CPU module.	—	—	Page 131 Start Communication
End communication	Ends communication with a CPU module.	—	—	Page 133 End Communication
1 shot communication	Executes functions set in the selected cell area at any timing.	—	—	Page 134 1 SHOT COMMUNICATION
Create button	Creates buttons to facilitate Start Communication, End Communication, and 1 Shot Communication operations.	—	—	Page 143 CREATING BUTTONS
Protect/Unprotect MX Sheet setting	Sets/Cancel the password for protecting the MX Sheet setting.	—	—	Page 149 PROTECTING/ UNPROTECTING MX Sheet SETTING
Options	Sets the output format of the "ErrorLog" sheet and the workbook protection during communication.	—	—	Page 152 OPTIONS
Setting data export	Outputs MX Sheet settings in CSV file format.	—	—	Page 156 EXPORTING SETTING DATA

*1 This number of device points refers to the case where word device data is collected/written in 16-bit integer.

The number of device points that can be set changes depending on the device data type, etc.

*2 Up to 100 cell areas can be set in one Excel file (one Excel book).

*3 Up to 1000 cell areas can be set in one Excel file (one Excel book).

*4 Only bit devices can be set.

*5 Up to 500 cell areas can be set in one Excel file (one Excel book).


3 CELL SETTING


This chapter explains cell setting required to operate MX Sheet.

3.1 Operation of "Cell Settings" Screen

This section explains the procedure for displaying the "Cell Settings" screen and changing the setting items. In the "Cell Settings" screen, its setting items change automatically depending on the selected function.

Window

[MX Sheet] tab ⇒ [Cell Setting] ()

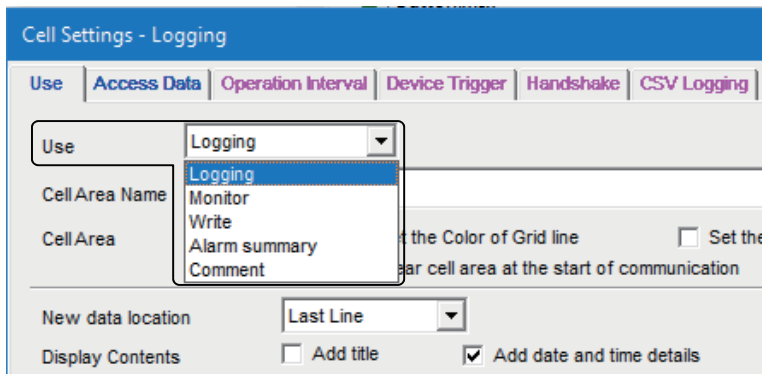


The setting of the "Cell Settings" screen can be changed by selecting "Use" of the [Use] tab. The following table shows the function outlines and relevant sections for options of "Use".

Item	Function	Reference
Logging	Set when using the logging function.	Page 47 When "Logging" is Selected
Monitor	Set when using the monitor function.	Page 83 When "Monitor" is Selected
Write	Set when using the write function.	Page 92 When "Write" is Selected
Alarm summary	Set when using the alarm summary function.	Page 100 When "Alarm Summary" is Selected
Comment	Set when using the comment display function.	Page 110 When "Comment" is Selected

Point

- Inverter communication/Robot controller communication is not supported other than "Logging".
- A system label^{*1} can also be set on the "Cell Settings" screen where a label can be set.

*1 There are two kinds of system labels; system label Ver.1 and system label Ver.2. For the differences between system label Ver.1 and system label Ver.2, refer to the HELP of MELSOFT Navigator. For their respective creation methods, refer to the following:
 MX Component Version 5 Reference Manual

3.2 When "Logging" is Selected

This section explains the "Cell Settings" screen when "Logging" is selected from "Use" of the [Use] tab.


Tab	Required/optional	Reference
[Use] tab	Required setting	☞ Page 48 Setting of the [Use] tab
[Access Data] tab	Required setting	☞ Page 55 Setting of the [Access Data] tab
[Operation Interval] tab	Required setting	☞ Page 61 Setting of the [Operation Interval] tab
[Device Trigger] tab	Optional setting	☞ Page 67 Setting of the [Device Trigger] tab
[Handshake] tab	Optional setting	☞ Page 69 Setting of the [Handshake] tab
[CSV Logging] tab	Optional setting	☞ Page 80 Setting of the [CSV Logging] tab

Setting of the [Use] tab

This section explains the setting of the [Use] tab for use of the logging function.

On the [Use] tab, set the cell area, logging data display position, displayed content, and operation when the cell is full.

Window

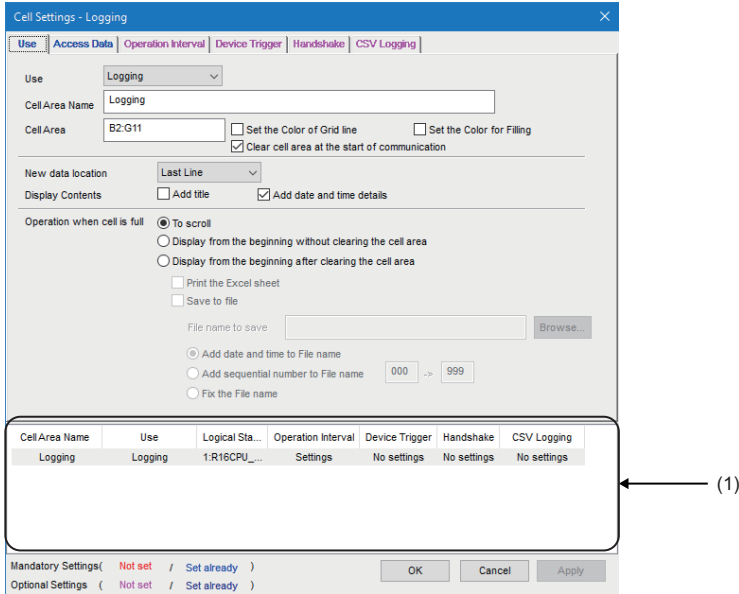

Displayed items


Item	Description	Reference
Use	Set the function to be used for the specified cell area. Select "Logging" when using the logging function.	—
Cell Area Name	Set the name of the specified cell area. (Maximum number of cell area names: 100)	
Cell Area	Enter the value to specify the cell area.	Page 49 "Cell Area"
Set the Color of Grid line	Select this checkbox to add grid lines (including color designation) to the specified cell area.	Page 50 "Set the Color of Grid line" and "Set the Color for Filling"
Set the Color for Filling	Select this checkbox to color the specified cell area.	
Clear cell area at the start of communication	Select this checkbox to clear the data of specified cell area at the start of communication. (Default: selected)	Page 50 "Clear cell area at the start of communication"
New data location	Set the latest data display position of the logging data. • Last Line The latest data is displayed at the last of the specified cell area. • First Line The latest data is displayed at the first of the specified cell area.	Page 51 "New data location"
Display Contents	Select a checkbox to add a title or date and time to the displayed logging data.	Page 52 "Display Contents"
Operation when cell is full	Set the operation to be performed when the specified cell area is full. • To scroll The displayed contents are scrolled and displayed. • Display from the beginning without clearing the cell area The data currently displayed in the cell area are overwritten and logging is resumed. Before logging is resumed, the Excel spreadsheet can be printed and saved. • Display from the beginning after clearing the cell area The data displayed in the cell area are erased and logging is resumed. Before logging is resumed, the Excel spreadsheet can be printed and saved.	Page 53 "Operation when cell is full"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Cell Area"


Set the cell area to be used by the logging function.

■Setting examples

When a single cell area is specified (B2 to D5)

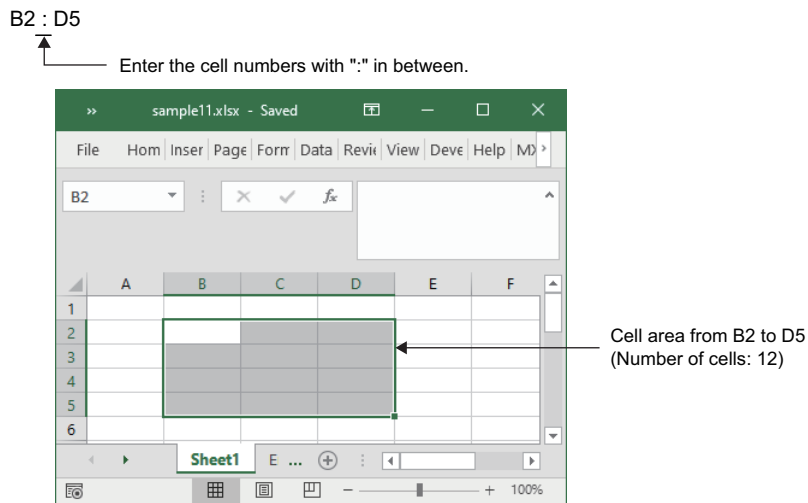

When multiple cell areas are specified (B2 to D5 (Specified cell area ❶) and B8 to D11 (Specified cell area ❷))

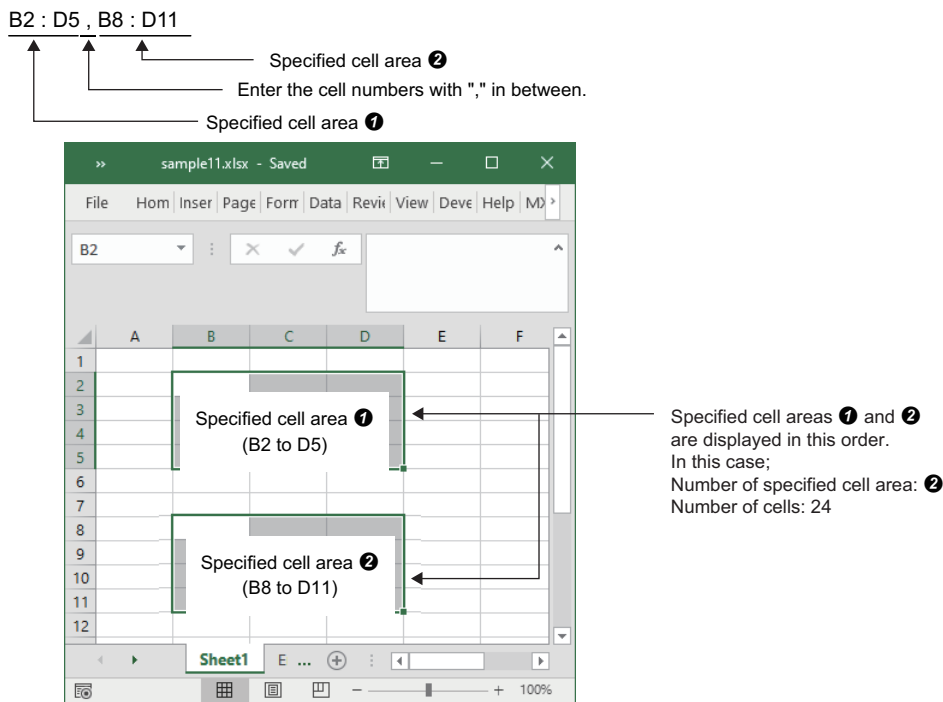

■Setting ranges

The following shows the available number of cells and the number of specified cell areas.


Item	Setting range
Cell	When date and time are added: 255 columns × 1000000 rows When date and time are not added: 256 columns × 1000000 rows
Number of specified cell areas	Up to 16

"Set the Color of Grid line" and "Set the Color for Filling"

Set the colors of cell area grid lines and cell filling.

Depending on the specified colors, all colors may turn to gray.

For details, refer to the following:

 Page 12 Considerations for setting MX Sheet

"Clear cell area at the start of communication"

Set whether or not to clear the data of cell area at the start of communication.

■ Display example in the case where the checkbox of "Clear cell area at the start of communication" is selected

- Before the start of communication

2021/03/25 Thu 13:00:00	15	37
2021/03/25 Thu 13:00:05	16	39
2021/03/25 Thu 13:00:10	17	42



- At the start of communication



- At the completion of the first collection

2021/03/25 Thu 15:00:00	31	102

■ Display example in the case where the checkbox of "Clear cell area at the start of communication" is not selected

- Before the start of communication

2021/03/25 Thu 13:00:00	15	37
2021/03/25 Thu 13:00:05	16	39
2021/03/25 Thu 13:00:10	17	42



- At the start of communication

2021/03/25 Thu 13:00:00	15	37
2021/03/25 Thu 13:00:05	16	39
2021/03/25 Thu 13:00:10	17	42



- At the completion of the first collection

2021/03/25 Thu 13:00:00	15	37
2021/03/25 Thu 13:00:05	16	39
2021/03/25 Thu 13:00:10	17	42
2021/03/25 Thu 15:00:00	31	102

"New data location"

Set the location of the latest data when using the logging function.

■ Display example in the case where "Last Line" is selected

2022/02/14 Mon 11:05:50	21	37	↑ Old data New data
2022/02/14 Mon 11:05:55	26	39	
2022/02/14 Mon 11:06:05	30	42	
2022/02/14 Mon 11:06:10	35	44	
2022/02/14 Mon 11:06:15	39	46	

■ Display example in the case where "First Line" is selected

2022/02/14 Mon 11:07:25	21	16	New data ↓ Old data
2022/02/14 Mon 11:07:20	17	13	
2022/02/14 Mon 11:07:15	12	11	
2022/02/14 Mon 11:07:10	8	9	
2022/02/14 Mon 11:07:05	3	6	

"Display Contents"

■ "Add title" checkbox

Set whether or not the date and time and the title for device name is displayed at the first line of the "Cell Area".
Select this check box to display the title.

Ex.

When the checkbox of "Add date and time details" is selected and the devices D100 to D103 are set

Title		D100	D101	D102	D103
Collection data	2021/05/21 Mon 13:24:14	30	100	0	37
	2021/05/21 Mon 13:24:17	40	80	0	55

The device name set on the [Access Data] tab is displayed.

Point

- The title line is not the target of cell area clear at the start of communication or clear when cell is full.
 - When the Cell Area is set at multiple locations, the title is displayed for only the Cell Area specified first.
- Example) When "B2:E4,B6:E8" is set for the Cell Area on the [Use] tab

	Date	D0	D1	D2
	2022/02/11 Fri 09:14:23	37	0	100
	2022/02/11 Fri 09:14:28	41	0	35
	2022/02/11 Fri 09:14:33	45	0	91
	2022/02/11 Fri 09:14:38	48	0	88
	2022/02/11 Fri 09:14:43	52	0	82

■ "Add date and time details" checkbox

Set whether or not to add the logging date and time to the cell area set in the "Cell Area".
Select this checkbox to add the date and time.

In this case, the leftmost column of the logging data area is used for the date and time. (One item of logging data decreases.)
The date and time column displays the date and time of the personal computer where MX Sheet is installed.

2021/05/23 Wed 18:31:06
(1) (2) (3)

(1) Indicates the date as "year/month/day".

(2) Indicates the day of the week as "Sun (Sunday), Mon (Monday), Tus (Tuesday), Wed (Wednesday), Thu (Thursday), Fri (Friday), Sat (Saturday)".

(3) Indicates the time as "hours: minutes: seconds".

Point

The above date and time can be edited on Excel.

However, if the cell setting is edited again after editing on Excel, the setting on Excel are invalid.


"Operation when cell is full"

Set the operation to be performed when the specified cell area is full of logging data.


When "New data location" is set to "First Line", "Display from the beginning without clearing the cell area" cannot be selected.

■When "To scroll" is selected

- When "New data location" is set for "Last Line"

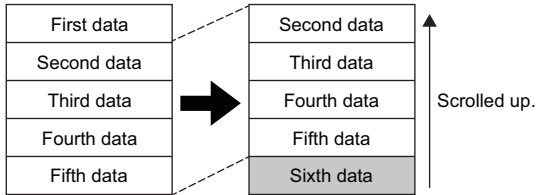


- When "New data location" is set for "First Line"

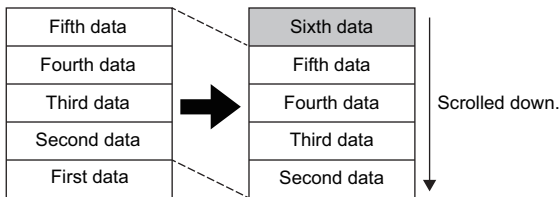


■When "Display from the beginning without clearing the cell area" is selected

When the cell is full, Excel spreadsheet print or Excel book save can also be performed.

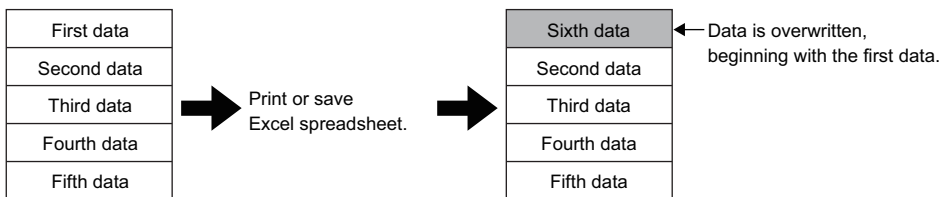

■When "Display from the beginning after clearing the cell area" is selected

When the cell is full, Excel spreadsheet print or Excel book save can also be performed.

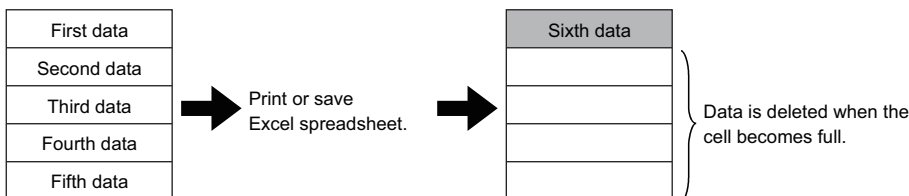

■When "Print the Excel sheet" is selected

The Excel spreadsheet is printed when the cell is full.

After completion of print, all data is erased and logging is resumed.

This item can be selected when "Display from the beginning without clearing the cell area" or "Display from the beginning after clearing the cell area" is selected for "Operation when cell is full".

■When "Save to file" is selected

The Excel book is saved when the cell is full.


After completion of save, all data is erased and logging is resumed.

This item can be selected when "Display from the beginning without clearing the cell area" or "Display from the beginning after clearing the cell area" is selected for "Operation when cell is full".

When selecting "Save to file", set the following settings for the file where data is saved.

Item	Description
File name to save	The storage location and file name are set for the Excel book to be saved when the cell is full.*1*2 The Excel file (.xls, .xlsx, .xlsm, .xlsb)*3, HTML file (.htm), or CSV file (.csv) can be set as the file type.*4
Add date and time to File name	The file set in "File name to save" saves data with the date and time added to its file name. The following shows a file name format when data is saved. <div style="text-align: center;"> <p>*****20210523183536.extension</p> <p>Extension set to "File name to save" Seconds Minutes Hours Day Month Year File name set in "File name to save"</p> </div>
Add sequential number to File name	The file set in "File name to save" saves data with a number added to its file name. A serial number can be set within the range from 000 to 999. When the number reaches to the last, the file of the first number is overwritten by the newly saving file. The following shows a file name format when data is saved. <div style="text-align: center;"> <p>*****000.extension</p> <p>Extension set in "File name to save" File number File name set in "File name to save"</p> </div>
Fix the File name	Data is overwritten to the file set in "File name to save."

*1 A UNC path name (\\server name\path name) cannot be specified as a file name. After assigning the network drive, specify the path name.

*2 For the continuous operation when saving data automatically in a file, refer to the following:
 Page 14 Continuous operation of Excel

*3 An Excel file can be set only with the same extension as the file in which MX Sheet is set.

*4 In the case of an Excel file or HTML file, the whole Excel book is saved. However, in the case of a CSV file, only the data of the target sheet is saved.

Preset cell areas


The cell areas already set to the Excel book are displayed.

The following operations are available by selecting the cell area name in the "preset cell areas".

■Reading the settings

Select and double-click the cell area name to read the settings of the selected cell area name to the "Cell Settings" screen.


■Deleting the settings

Select the cell area name and press the  key to erase all the settings of the selected cell area name.

Setting of the [Access Data] tab

On the [Access Data] tab, set the logical station number required for communication with a CPU module and the device data to be collected in the cell area.

Window

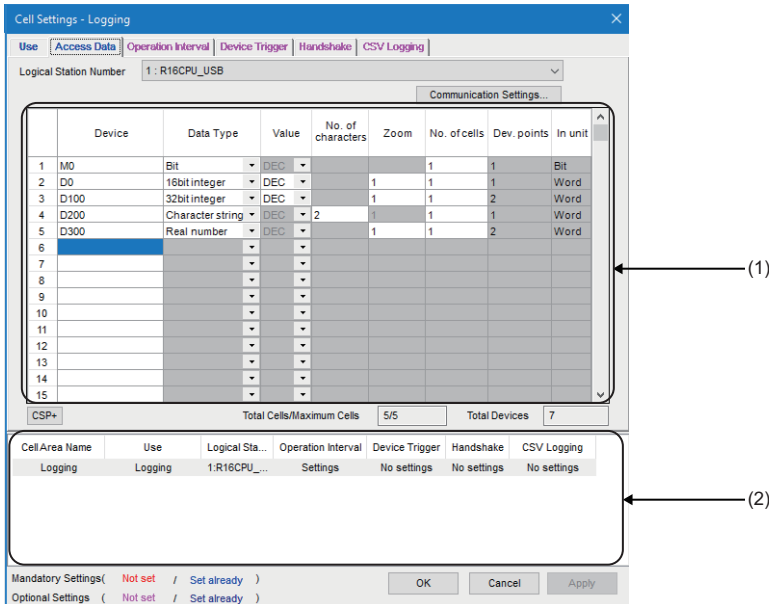

Displayed items

Item	Description	Reference
Logical Station Number	Select the logical station number required for communication.	Page 55 "Logical Station Number"
[Communication Settings] button	Click this to start Communication Settings Utility for setting a new logical station number and changing settings.	Page 56 [Communication Settings] button
Remote password*1	Enter the password when the password is set to the connection target CPU module.	Page 56 "Remote password"
(1) (Access data)	Set the devices or labels to be logged.	Page 56 Access data
[CSP+] button	Click this to display the "Getting CSP+ for machine" screen.	Page 60 Importing CSP+ for machine
Total Cells/Maximum Cells	The number of cells for which a device is set in a cell area/the number of cells that can be set in the area is displayed.	—
Total Devices	The number of device points set in the cell area is displayed.	—
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

*1 "Remote password" is displayed when the logical station number selected in "Logical Station Number" on the [Access Data] tab is the one for the password function compatible module.

"Logical Station Number"

Select the logical station number required for communication.

If the logical station number is already set, the number is displayed in the list box and can be selected.

If the logical station number is not set, click the [Communication Settings] button and set a new logical station number.

[Communication Settings] button

Click this to start Communication Settings Utility for setting a new logical station number and changing settings.

Select "Run as administrator" when the "User Account Control" (Page 176 Warning Messages on Windows) screen asking if execute programs with administrator authority or not appears.

After starting Communication Settings Utility, click the [Wizard] button and set a new logical station number and change the settings with Communication Setting Wizard.

For the detailed explanation of Communication Settings Utility and Communication Setting Wizard, refer to the following:

MX Component Version 5 Reference Manual

"Remote password"

The "Remote password" screen is displayed when the setting of the logical station number selected in "Logical Station Number" includes information on the connection to the module with the password function.

Enter the password when the password is set to the connection target CPU module.

It need not be entered when the password is not set.

Access data

Order of display

Data is displayed in the cell area in the order of the numbers shown on the left of the [Access Data] tab.

- Device data display example

Setting example of the [Access Data] tab

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	D0	16bit integer	DEC		1	3	3	Word
2	W0	16bit integer	DEC		1	3	3	Word
3	B0	Bit	DEC			3	3	Bit

Data numbers

The device data is displayed on Excel as shown below.

	D0	D1	D2	W0	W1	W2	B0	B1	B2
1									
2	Date time								
3	2022/02/25 Fri 16:19:24	18	14	0	0	0	0	0	0

Data No. 1 Data No. 2 Data No. 3

Displayed in order of data numbers.

"Device"

Enter a device or label to be accessed.

- When entering a device, enter in the order of a device name and device number.
- When entering a label, enter the label name.
- The applicable data types are Bit and Word.
- When entering a label, enter other than structured data type label and array type label.

For the accessible devices, refer to the following:

Page 19 Accessible range

■"Data Type"

Set the data type to be displayed in the cell.

Item	Available Device	Description
Bit	Bit device	Bit devices set in "Device" are displayed in a single cell in units of one bit.
	Word device (Bit specification)	Designated bits for word device set in "Device" are displayed in a single cell in units of one bit (e.g. D0.0).
16 bit integer (-32768 to 32767)	Bit device ^{*1}	Displayed in a single cell in units of 1 word (16 bits), starting with the 16 bit integer device number set in "Device". ^{*2}
	Word device	Displayed in a single cell in units of 1 word, starting with the device number set in "Device". ^{*2}
32 bit integer (-2147483648 to 2147483647)	Bit device ^{*1}	Displayed in a single cell in units of 2 words (32 bits), starting with the device number set in "Device". ^{*2}
	Word device	Displayed in a single cell in units of 2 words, starting with the device number set in "Device". ^{*2}
	Double word device	Data of device number set to "Device" are displayed in a single cell in units of 1 device (32-bit). ^{*2}
	Monitor type	Monitor types set in "Device" are displayed in a single cell in units of 2 words. ^{*2}
Character string	Bit device ^{*1}	Data of the device number set in "Device" are displayed in the cell as character strings. ^{*3}
	Word device	Data of the device number set in "Device" are displayed in the cell as character strings. ^{*3}
Real number ^{*4} ($\pm 2^{-126} \leq \text{value} < \pm 2^{128}$, 0)	Bit device ^{*1}	Displayed in a single cell in units of 2 words (32 bits), starting with the device number set in "Device". ^{*2}
	Word device	Displayed in a single cell in units of 2 words, starting with the device number set in "Device". ^{*2}

*1 Displayed in a single cell in units of one bit for R motion CPU and Q motion CPU.

*2 The displayed value changes depending on the "Zoom" setting. (☞ Page 59 "Zoom")

*3 The unit and the number of displayed characters of the read data change depending on the "No. of characters" setting. (☞ Page 58 "No. of characters")

*4 A single-precision floating point data type. The number of significant digits in MX Sheet is seven, and the eighth digit is rounded off to be displayed in a cell.

■"Value"

Select the display format of the value to be displayed in the cell from DEC and HEX.

Depending on the "Data Type", the "Value" and "Zoom" can be selected/set as shown below.

Item			Cell data display
Data type	Value	Zoom	
Bit	Not applicable	Not applicable	0 or 1
16 bit integer	DEC	Applicable	Displayed in decimal
	HEX	Not applicable	Displayed in 4-digit hexadecimal (Example: 03EB)
32 bit integer	DEC	Applicable	Displayed in decimal
	HEX	Not applicable	Displayed in 8-digit hexadecimal (Example: 03EB03EA)
Character string	Not applicable	Not applicable	Character string is displayed (Example: ABCD)
Real number	Not applicable	Applicable	Real number is displayed (Example: 1.36E-36)

■ "No. of characters"

Set the number of characters to be displayed in a single cell.

Setting range: 40

Depending on the value set in "No. of characters" and device data, the character strings may not be displayed in the cell. The following are the examples of setting 1 to 4 in "No. of characters".

Ex.

When displaying the character strings stored in D0 to D3


	b15 to b8	b7 to b0
D0	B	A
D1	D	C
D2	F	E
D3	H	G

- When "No. of characters" is set to "1"

The data is displayed in a single cell in units of 1 word (16 bits).

Only the character stored in b0 to b7 of D0 is displayed.


The character stored in b8 to b15 of D0 is not displayed.



- When "No. of characters" is set to "2"

The data is displayed in a single cell in units of 1 word (16 bits).

The character strings stored in b0 to b7 and b8 to b15 are displayed in this order.




- When "No. of characters" is set to "3"

The data is displayed in a single cell in units of 2 words (32 bits).

The character strings stored in D0 (b0 to b7, b8 to b15) and D1 (b0 to b7) are displayed.


The character string stored in b8 to b15 of D1 is not displayed.



- When "No. of characters" is set to "4"

The data is displayed in a single cell in units of 2 words (32 bits).

The character strings stored in D0 (b0 to b7, b8 to b15) and D1 (b0 to b7, b8 to b15) are displayed in this order.




■"Zoom"

The device value read from a CPU module is multiplied by the zoom ratio and displayed in the cell.

When "Data Type" is set to "Bit" or "Character string" or when "Value" is set to "HEX", "Zoom" cannot be set.

Setting range: 0.001 to 1000

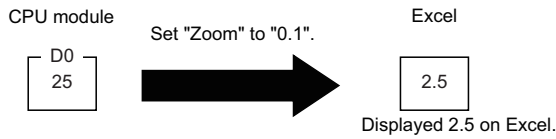

■"No. of cells"

Set the number of cells to be used for the device set in "Device" within the area specified in "Cell Area".

When the system labels are specified to devices and inverter communication setting/robot controller communication setting is set to the logical station number, '1' is displayed.

- Device data display example

Setting example of the [Access Data] tab

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	D0	16bit integer	DEC		1	3	3	Word
2								
3	Device: D0							
4	Data Type: 16bit integer							
5	No. of cells: 3							
6								

The device data is displayed on Excel as shown below.

Date time	D0	D1	D2			
2022/2/11 Fri 10:03:10	0	0	0			

3 points are displayed in order, starting with D0. These are set as the cell area but not used.

■"Dev. Points"

The points of the devices to be consecutively read starting with the device number set in "Device" are displayed.

When inverter communication setting/robot controller communication setting is set to the logical station number, '2' is displayed.

■"In unit"


The unit of the device to be shown in the cell is displayed.

When inverter communication setting/robot controller communication setting is set to the logical station number, "Word" is displayed.

Importing CSP+ for machine

Set device data in a batch by importing CSP+ for machine.

Window

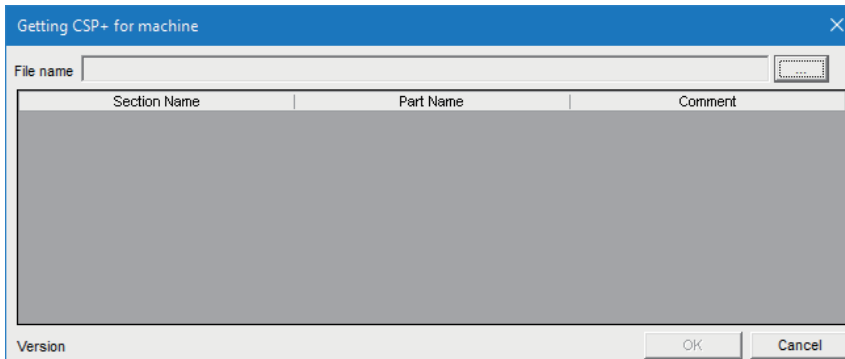

Displayed items

Item	Description						
File name	The name of CSP+ for machine is displayed.						
[...] button	Click this to display the screen for selecting CSP+ for machine. Select CSP+ for machine to import, and click the [OK] button.						
(1) (Section part list)	<table border="1"> <tr> <td>Section Name</td> <td>The LABEL of COMM_IF^{*1} of CSP+ for machine is displayed.</td> </tr> <tr> <td>Part Name</td> <td>The LABEL of COMM_IF_VARIABLE^{*1} of CSP+ for machine is displayed. For devices without this item are not displayed in this list.</td> </tr> <tr> <td>Comment</td> <td>The COMMENT of COMM_IF_VARIABLE^{*1} of CSP+ for machine is displayed.</td> </tr> </table>	Section Name	The LABEL of COMM_IF ^{*1} of CSP+ for machine is displayed.	Part Name	The LABEL of COMM_IF_VARIABLE ^{*1} of CSP+ for machine is displayed. For devices without this item are not displayed in this list.	Comment	The COMMENT of COMM_IF_VARIABLE ^{*1} of CSP+ for machine is displayed.
Section Name	The LABEL of COMM_IF ^{*1} of CSP+ for machine is displayed.						
Part Name	The LABEL of COMM_IF_VARIABLE ^{*1} of CSP+ for machine is displayed. For devices without this item are not displayed in this list.						
Comment	The COMMENT of COMM_IF_VARIABLE ^{*1} of CSP+ for machine is displayed.						
Version	The file version of CSP+ for machine is displayed.						

*1 Check the setting value of COMM_IF and COMM_IF_VARIABLE with CSP+ for machine creation support tool. CSP+ for machine creation support tool can be downloaded from the CC-Link Partner Association website (www.cc-link.org/en/index.html).


Operating procedure

1. Click the [...] button, and select target CSP+ for machine.
2. Select a combination of a section and a part to set device data in Section part list, and click the [OK] button. Device data of the selected section and part is set for the access data in the [Access Data] tab in a batch.

Setting of the [Operation Interval] tab

This section explains the setting of the [Operation Interval] tab for use of the logging function.
 On the [Operation Interval] tab, set the day, time and time zone of the activation of the function for the cell area.

Window

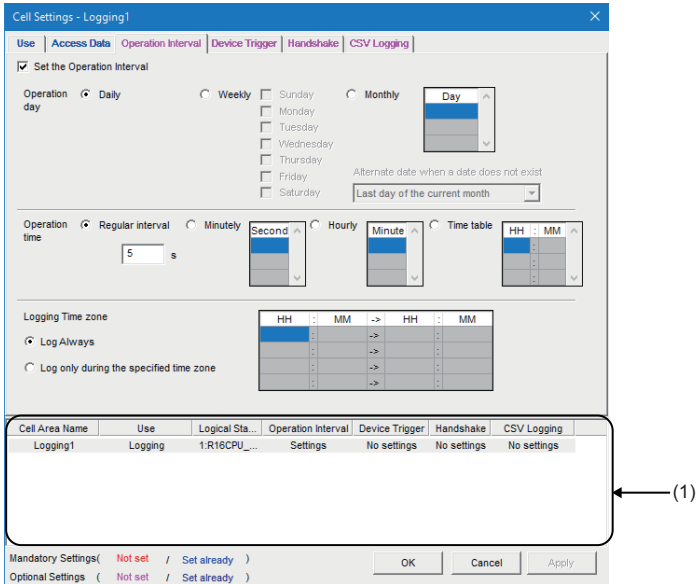

Displayed items

Item	Description	Reference
Set the Operation Interval	Set the operation of the cell area valid or invalid.	Page 62 "Set the Operation Interval"
Operation day	Set the operation day of the logging activation.	Page 62 "Operation day"
Operation time	Set the operation time of the logging activation.	Page 63 "Operation time"
Logging Time zone	Set the time zone of the logging activation.	Page 64 "Logging Time zone"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Set the Operation Interval"

To set the settings of cell area invalid or to use the function of cell area for 1 shot communication only, clear the check box.
(Do not clear the check mark for the case of ordinary operation.)

"Operation day"

Set the operation day of device data collection.

■When "Daily" is selected

Operation is performed every day.

■When "Weekly" is selected

Operation is performed on the specified day of the week only.

Multiple days of the week can be set.

■When "Monthly" is selected

Operation is performed on the specified days only.

If the specified day does not exist in some months, an alternate day can be specified.

Number of days that can be set: 31

- When "15th" is set

Operation is performed on the 15th of every month, e.g. January 15, February 15, March 15.

- When "31st" is set

Excepting February, April, June, September and November, operation is performed on the 31st every month.

For February, April, June, September and November, set the alternate day and processing in "Alternate day when a date does not exist".

The following table shows the setting items of "Alternate day when a date does not exist".

Item	Description
Last day of the current month	Operation is performed on the last day of February, April, June, September or November.
First day of the next month	Operation is performed on the first day of the next month.
No operation	Operation is not performed in February, April, June, September and November.

"Operation time"

Set the operation time of device data collection.

■When "Regular interval" is selected

Device data is collected at the set second intervals.

When setting lesser "seconds" than the actual communication time, the fixed interval communication cannot be established. Hence, set for longer than the actual communication time.

For Communication time, refer to the following performance value.

☞ Page 161 Processing Speed of MX Sheet

Setting range: 0.001 to 0.999 (in units of 0.001 seconds), 1 to 3600 (in units of 1 second)

When the date and time are added, the date and time displayed on the Excel spreadsheet is in the "yyyy/mm/ dd ddd hh:mm:ss" format if the setting is 0.001 to 0.999 seconds.

Ex.

When 0.2 seconds interval is set

Date	D0	D1	D2
2022/02/11 Fri 10:20:19	37	0	100
2022/02/11 Fri 10:20:20	45	0	94
2022/02/11 Fri 10:20:20	56	0	83
2022/02/11 Fri 10:20:20	67	0	78
2022/02/11 Fri 10:20:20	78	0	62
2022/02/11 Fri 10:20:20	89	0	55
2022/02/11 Fri 10:20:21	101	0	43

■When "Minutely" is selected

Device data is collected at the specified second every minute.

Number of times that can be set: 60

■When "Hourly" is selected

Device data is collected at the specified minute every hour.

Number of times that can be set: 60

■When "Time table" is selected

Device data is collected at the specified time.

Number of times that can be set: 50

"Logging Time zone"

Set the time zone for logging.

■When "Log Always" is selected

Logging is always performed at the specified operation time of the operation day.

■When "Log only during the specified time zone" is selected

Logging is performed in the specified time zone only.

Number of settings: 4


When "Operation day" is set to "Weekly" or "Monthly", do not set the time zone that spans over a day as shown in below:

HH	:	MM	->	HH	:	MM
22	:	00	->	08	:	00
.	:	.	->	.	:	.
.	:	.	->	.	:	.
.	:	.	->	.	:	.

Setting examples


■ When performing data logging always

- Setting example

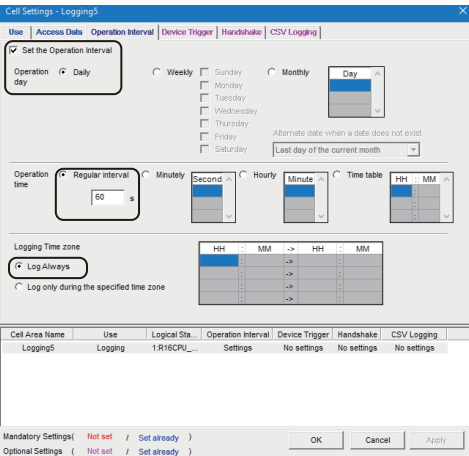


Item	Setting
Set the Operation Interval	Selected
Operation day	Daily
Operation time	Regular interval
	Time table
Logging Time zone	Log Always

- Operation timing

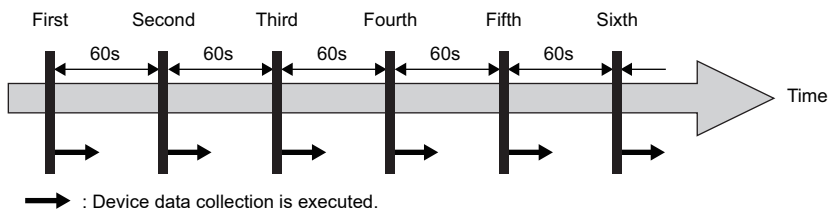


■ When performing data logging only during the specified time zone

• Setting example

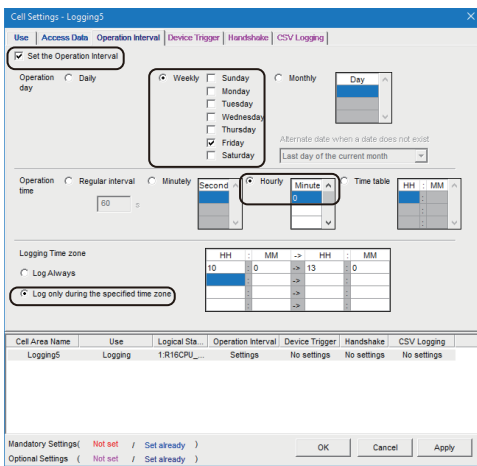

Item	Setting
Set the Operation Interval	Selected
Operation day	Weekly
	Friday
Operation time	Hourly
	Time table
	0 minutes
Logging Time zone	Log only during the specified time zone
	Time zone
	10:00 to 13:00


• Operation timing

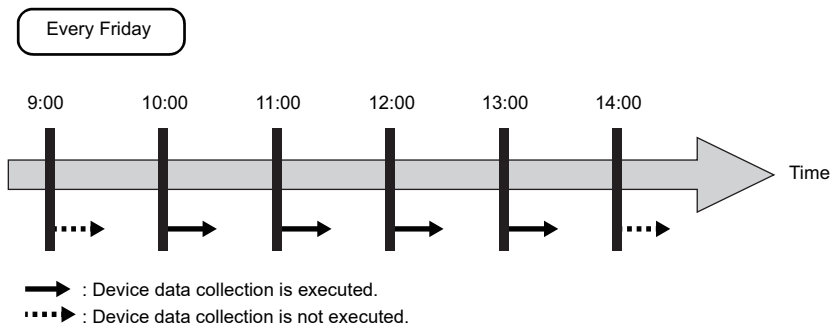

Setting of the [Device Trigger] tab

This section explains the setting of the [Device Trigger] tab for use of the logging function.
On the [Device Trigger] tab, set the device conditions for the device trigger.

Window

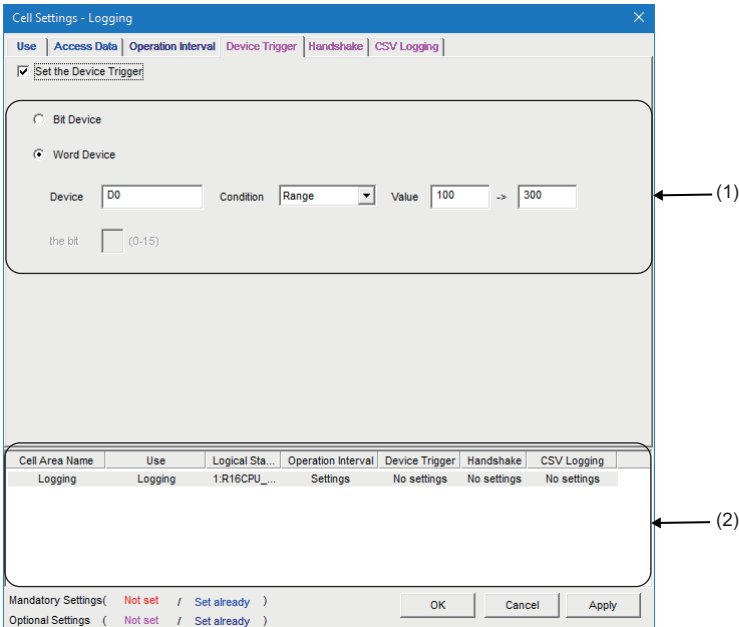

Displayed items

Item	Description	Reference
Set the Device Trigger	Set when the device trigger is used.	Page 67 "Set the Device Trigger"
(1) (Device conditions)	Set the device or label conditions.	Page 67 Device conditions
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Set the Device Trigger"

Be sure to select the checkbox of "Set the Device Trigger" to use the device trigger.

Device conditions

Set the device conditions for the device trigger.

■ Device type

Set the type of the device used for the device trigger.

Item	Description
Bit device	Set when using a bit device for the device trigger.
Word device	Set when using a word device or double word device for the device trigger, or the inverter communication setting/robot controller communication setting is set to the logical station number.

■ "Device"

Enter the device or label used for the device trigger.

- When entering a device, enter in the order of a device name and device number.
- When entering a label, enter the label name.
- The applicable data types are Bit and Word.
- When entering a label, enter other than structured data type label and array type label.





■"the bit"

Set the corresponding bit of the word device.

Setting range: 0 to 15

■"Condition"

Set the device trigger condition.

Item	Available Device	Description
When ON ON OFF 	Bit device	Set when operation is to be performed only once when the bit device turns ON.
	Word device	Set when operation is to be performed only once when the corresponding bit of the word device turns ON (value: 1).
When OFF ON OFF 	Bit device	Set when operation is to be performed only once when the bit device turns OFF.
	Word device	Set when operation is to be performed only once when the corresponding bit of the word device turns OFF (value: 0).
ON ON OFF 	Bit device	Set when operation is to be performed while the bit device is ON.
	Word device	Set when operation is to be performed while the corresponding bit of the word device is ON (value: 1).
OFF ON OFF 	Bit device	Set when operation is to be performed while the bit device is OFF.
	Word device	Set when operation is to be performed while the corresponding bit of the word device is OFF (value: 0).
=	Word device, Double word device	Set when operation is to be performed when the device value is equal to the "Value" setting.
<>	Word device, Double word device	Set when operation is to be performed when the device value is not equal to the "Value" setting.
<=	Word device, Double word device	Set when operation is to be performed when the device value is equal to or less than the "Value" setting.
<	Word device, Double word device	Set when operation is to be performed when the device value is less than the "Value" setting.
>=	Word device, Double word device	Set when operation is to be performed when the device value is equal to or greater than the "Value" setting.
>	Word device, Double word device	Set when operation is to be performed when the device value is greater than the "Value" setting.
Range	Word device, Double word device	Set when operation is to be performed when the device value is within the specified "Value" setting range.

■"Value"

Enter the values used for "Condition".


Setting range:

- Word device (-32768 to 32767)
- Double word device (-2147483648 to 2147483647)
- When inverter communication setting/robot controller communication setting (-2147483648 to 2147483647)

Ex.

When "Range" is to "Condition"


Enter the values in "Value" as shown below.

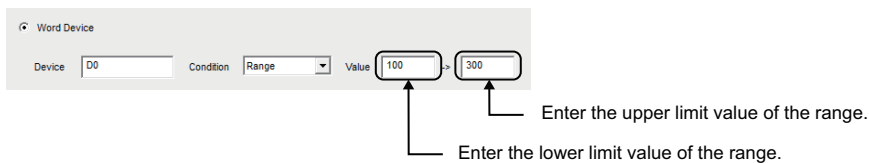

Setting of the [Handshake] tab

This section explains the setting of the [Handshake] tab for use of the logging function. On the [Handshake] tab, set the handshake requesting source and handshake processing.

Window

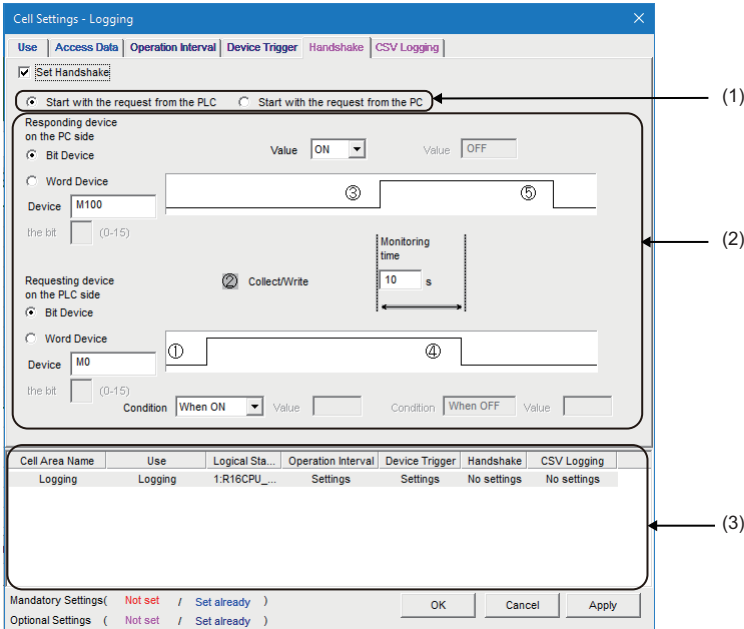

Displayed items

Item	Description	Reference
Set Handshake	Set when using a handshake.	Page 74 "Set Handshake"
(1) (Requesting source setting)	Set the requesting source of the handshake.	Page 74 Requesting source setting
(2) (Handshake processing)	Set the handshake processing.	Page 74 Handshake processing
(3) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Point


When inverter communication setting or Robot controller communication setting is set to the logical station number, handshake is not supported.

Setting examples and operation timing

The following shows the handshake setting examples and operation timing.


■ When "Start with the request from the PLC" is selected (Device: Bit device)

• Setting example

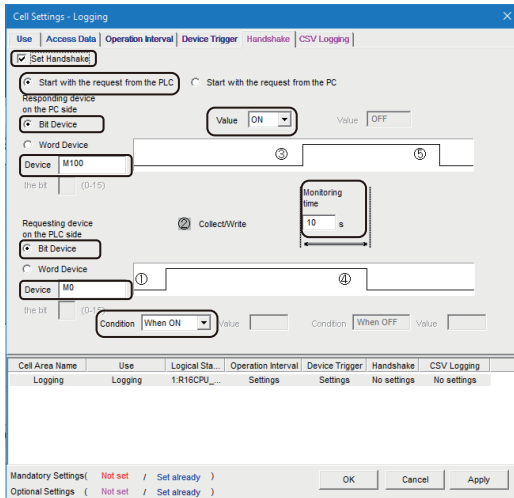

Item	Setting	
Set Handshake	Selected	
Start with the request from the PLC	Selected	
Responding device on the PC side	Bit Device	Selected
	Device	M100
	Value	ON
Requesting device on the PLC side	Bit Device	Selected
	Device	M0
	Condition	When ON
Monitoring time	10 seconds	


• Operation timing

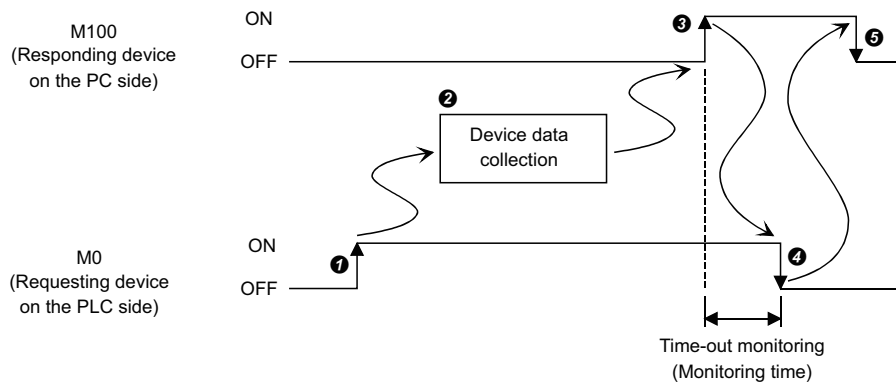

- ① When M0 turns ON, processing in ② is started.
- ② Device data is collected.
- ③ After device data is collected, M100 is turned ON.
- ④ M0 is turned OFF.
- ⑤ M100 is turned OFF.


■ When "Start with the request from the PLC" is selected (Device: Word device)

• Setting example

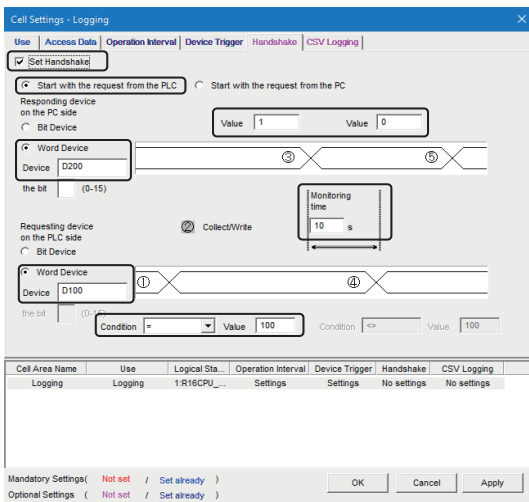

Item	Setting	
Set Handshake	Selected	
Start with the request from the PLC	Selected	
Responding device on the PC side	Word Device	Selected
	Device	D200
	Value	1 (left), 0 (right)
Requesting device on the PLC side	Word Device	Selected
	Device	D100
	Condition	=
	Value	100
Monitoring time	10 seconds	


• Operation timing

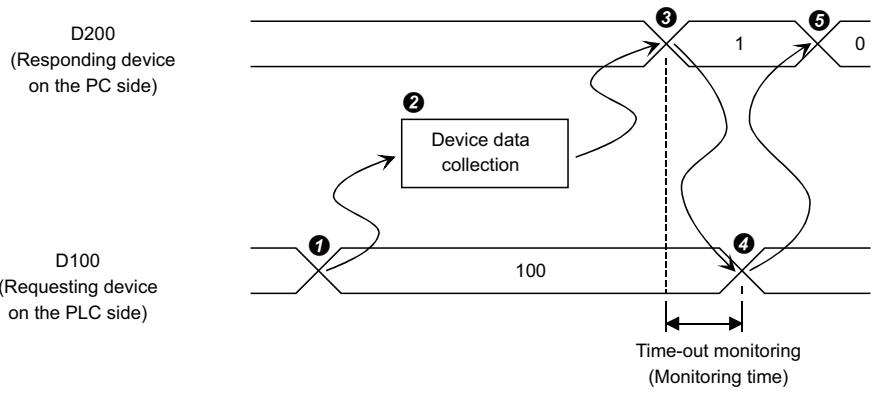

- ① When the D100 value reaches 100, processing in ② is started.
- ② Device data is collected.
- ③ After device data is collected, the D200 value is changed to 1.
- ④ The D100 value is changed to other than 100.
- ⑤ The D200 value is changed to 0.


■ When "Start with the request from the PC" is selected (Device: Bit device)

• Setting example

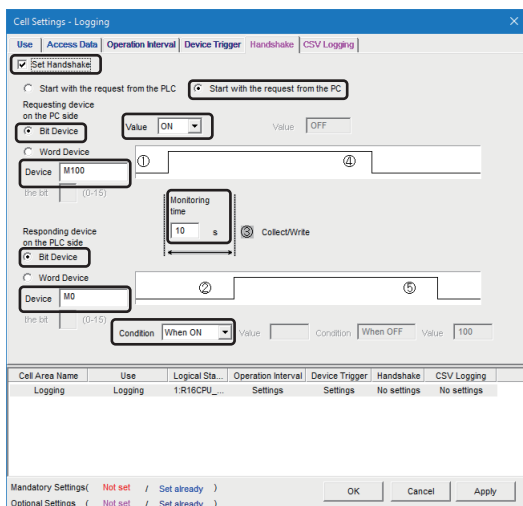

Item	Setting	
Set Handshake	Selected	
Start with the request from the PC	Selected	
Requesting device on the PC side	Bit Device	Selected
	Device	M100
	Value	ON
Responding device on the PLC side	Bit Device	Selected
	Device	M0
	Condition	When ON
Monitoring time	10 seconds	

• Operation timing

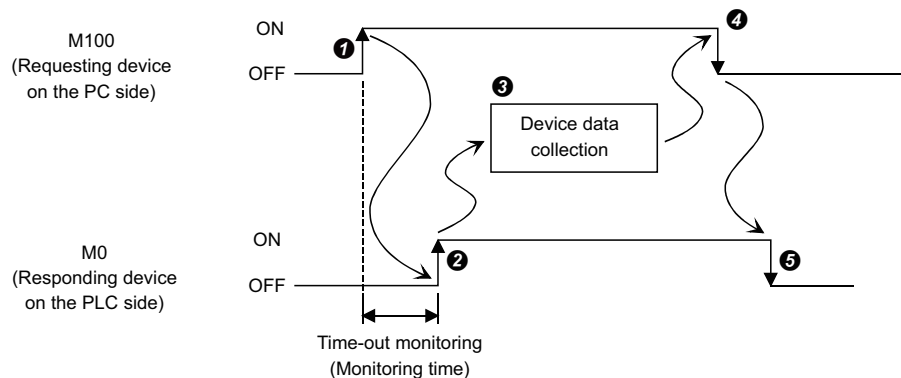

- ① M100 is turned ON.
- ② When M0 turns ON, processing in ③ is started.
- ③ Device data is collected.
- ④ After device data is collected, M100 is turned OFF.
- ⑤ M0 is turned OFF.


Point

Time-out monitoring is not executed between ④ and ⑤ above.

If the operation in ⑤ is not performed in a CPU module, device data collection is not executed when the handshake conditions are satisfied at the next time.


■ When "Start with the request from the PC" is selected (Device: Word device)

• Setting example

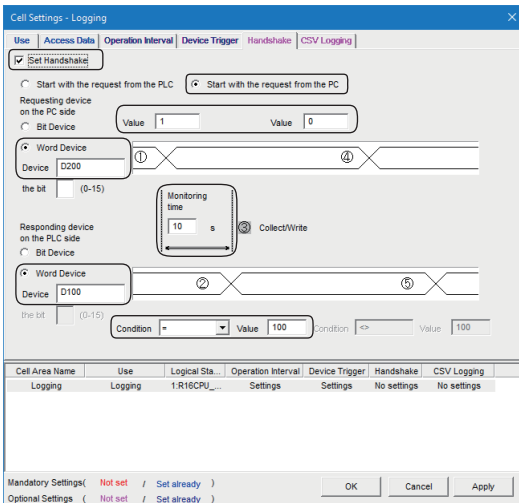

Item	Setting	
Set Handshake	Selected	
Start with the request from the PC	Selected	
Requesting device on the PC side	Word Device	Selected
	Device	D200
	Value	1 (left), 0 (right)
Responding device on the PLC side	Word Device	Selected
	Device	D100
	Condition	=
	Value	100
Monitoring time	10 seconds	

• Operation timing

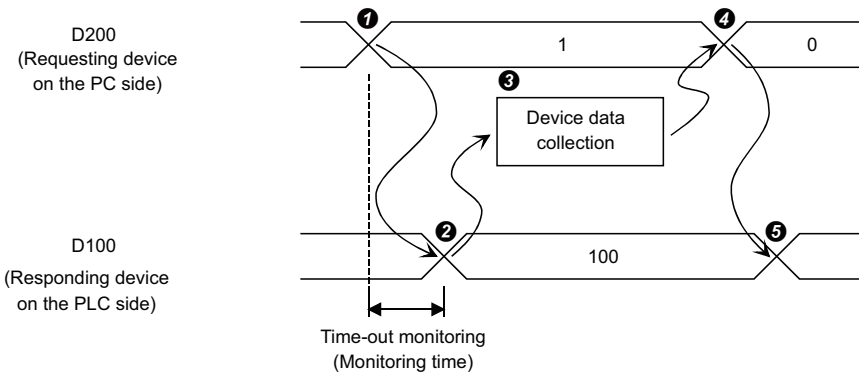

- ① The D200 value is changed to 1.
- ② When the D100 value reaches 100, processing in ③ is started.
- ③ Device data is collected.
- ④ After device data is collected, the D200 value is changed to 0.
- ⑤ The D100 value is changed to other than 100.

Point

Time-out monitoring is not executed between ④ and ⑤ above.
 If the operation in ⑤ is not performed in a CPU module, device data collection is not executed when the handshake conditions are satisfied at the next time.

"Set Handshake"

Be sure to select the checkbox of "Set Handshake" to use a handshake.

Requesting source setting

Set the requesting source for a device data collection start.

Item	Description
Start with the request from the PLC	Set when starting device data collection at the request of a CPU module.
Start with the request from the PC	Set when starting device data collection at the request of the personal computer.

Handshake processing

Set the handshake processing on a personal computer side and CPU module side.

■PC side processing

- Device type

Set the device type used for PC side processing.

Item	Description
Bit device	Set when a bit device is used for PC side processing.
Word device	Set when a word device or double word device is used for PC side processing.

- "Device"

Enter the device or label used for PC side processing.

·When entering a device, enter a device name and device number in this order.

·When specifying a bit of the word device, enter the bit number in "the bit".

·Bit cannot be specified for a double word device.

·When entering a label, enter the label name.

·The applicable data type is Bit.

·When entering a label, enter other than structured data type label and array type label.

- "Value"

Set the value of the device used for PC side processing.

Item	Available Device	Description
ON	Bit device	Set when the value of the device used for PC side processing is set for ON.
	Word device (Bit specification)	
OFF	Bit device	Set when the value of the device used for PC side processing is set for OFF.
	Word device (Bit specification)	
Empty (Value input)	Word device	Set the value of the word device used for PC side processing.
	Double word device	Set the value of the double word device used for PC side processing.

Setting range:

- Word device (-32768 to 32767)
- Double word device (-2147483648 to 2147483647)

■ CPU module side processing

- Device type

Set the device type used for CPU module side processing.

Item	Description
Bit device	Set when a bit device is used for CPU module side processing.
Word device	Set when a word device or double word device is used for CPU module side processing.

- "Device"

Enter the device or label used for CPU module side processing.

- When entering a device, enter a device name and device number in this order.
- When specifying a bit of the word device, enter the bit number in "the bit".
- Bit cannot be specified for a double word device.
- When entering a label, enter the label name.
- The applicable data type is Bit.
- When entering a label, enter other than structured data type label and array type label.

- "Condition"

Set the conditions of the device used for CPU module side processing.

Item	Available Device	Description
ON	Bit device	Set when the value of the device used for CPU module side processing is set for ON.
	Word device (Bit specification)	
OFF	Bit device	Set when the value of the device used for CPU module side processing is set for OFF.
	Word device (Bit specification)	
=	Word device, Double word device	Set when a CPU module side device value is equal to the "Value" setting.

- "Value"

Set the value of the device used for a CPU module processing.

This can be set only when "=" is selected in "Condition".

Setting range:

- Word device (-32768 to 32767)
- Double word device (-2147483648 to 2147483647)

■ Monitoring time

Set the time during which the PC side device monitors a CPU module side device.

Setting range: 1 to 3600

The monitoring time changes depending on the requesting source setting.


The following table shows the monitoring time.

Requesting Source Setting	Monitoring item
Start with the request from the PLC	Monitoring is executed from the time when the "PC side responding device" is set to the time when the "programmable controller side requesting device" is reset. If the "programmable controller side responding device" is not reset after the elapse of the monitoring time, the collected device data is discarded and the error log is displayed on the "ErrorLog" sheet.
Start with the request from the PC	Monitoring is executed from the time when the "PC side requesting device" is set to the time when the "programmable controller side responding device" is set. If the "programmable controller side requesting device" is not set after the elapse of the monitoring time, the error log is displayed on the "ErrorLog" sheet.


Sample ladders for handshake

The following shows the sample ladders for handshake used in the settings (Page 70 Setting examples and operation timing).

■When "Start with the request from the PLC" is selected (Device: Bit device)

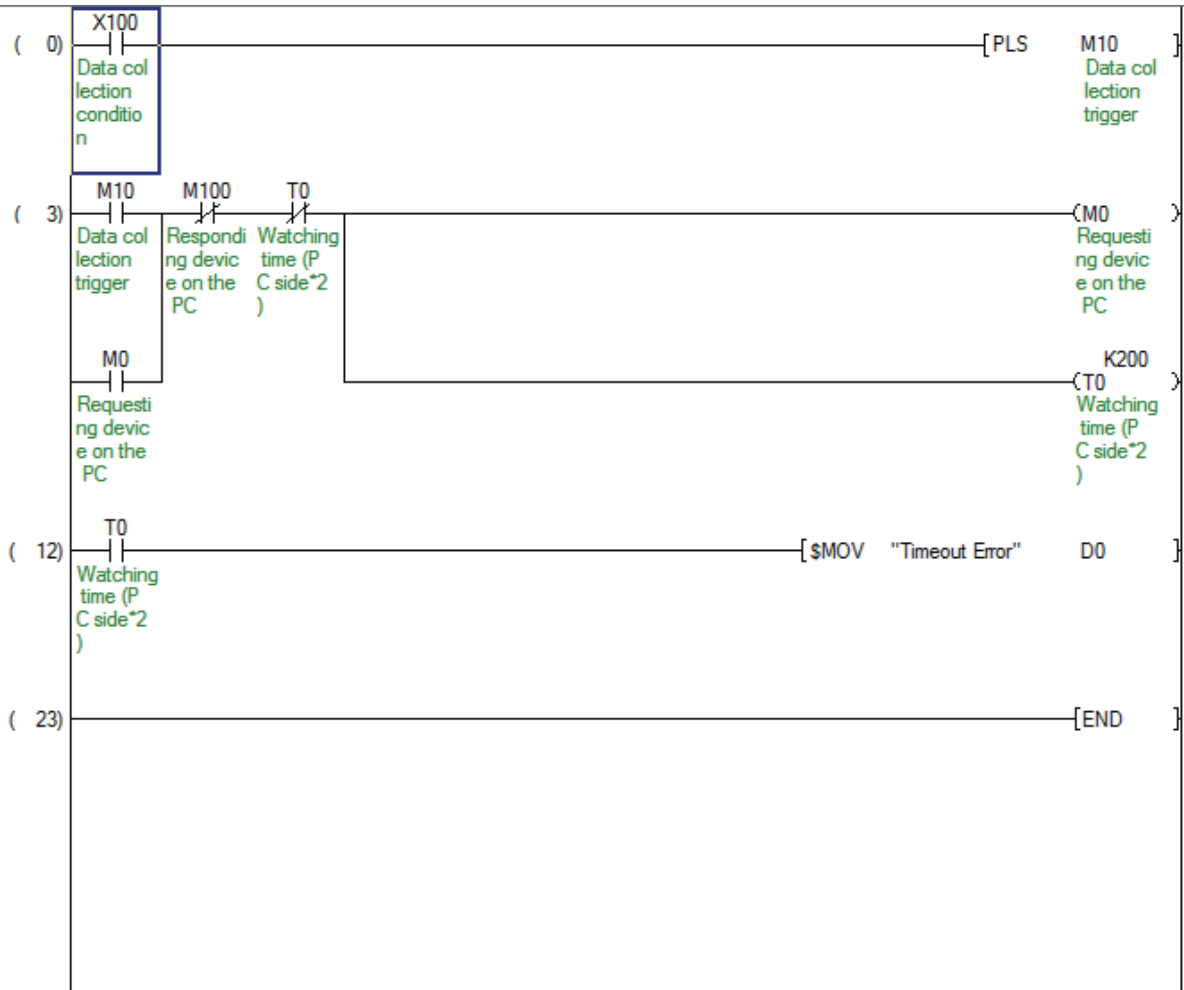


■When "Start with the request from the PLC" is selected (Device: Word device)

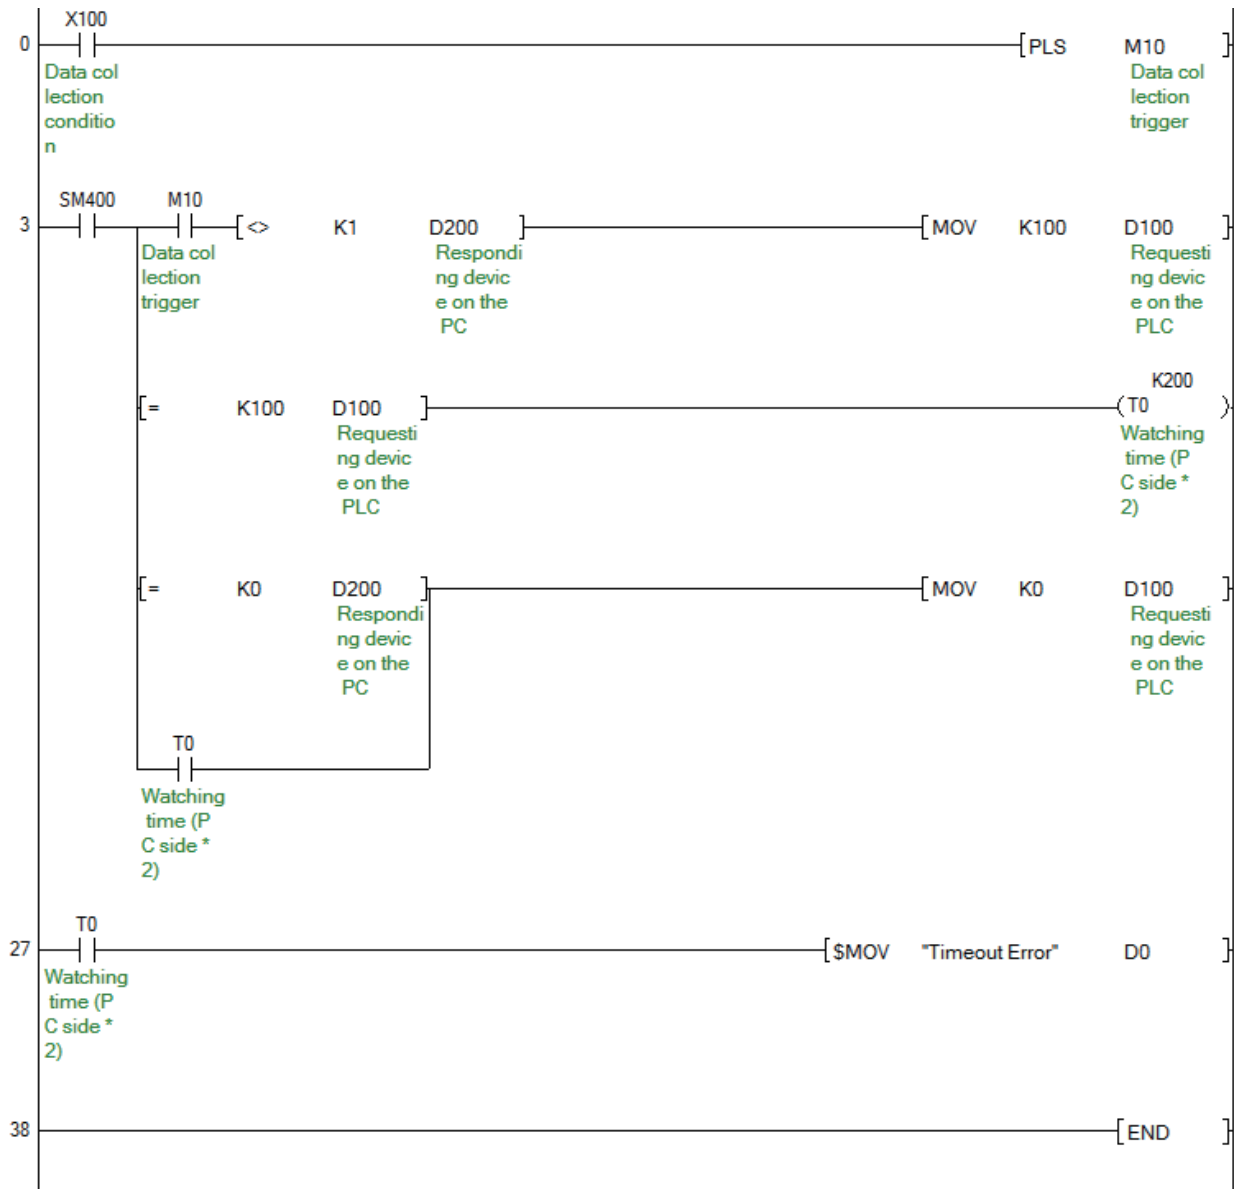


3

■When "Start with the request from the PC" is selected (Device: Bit device)

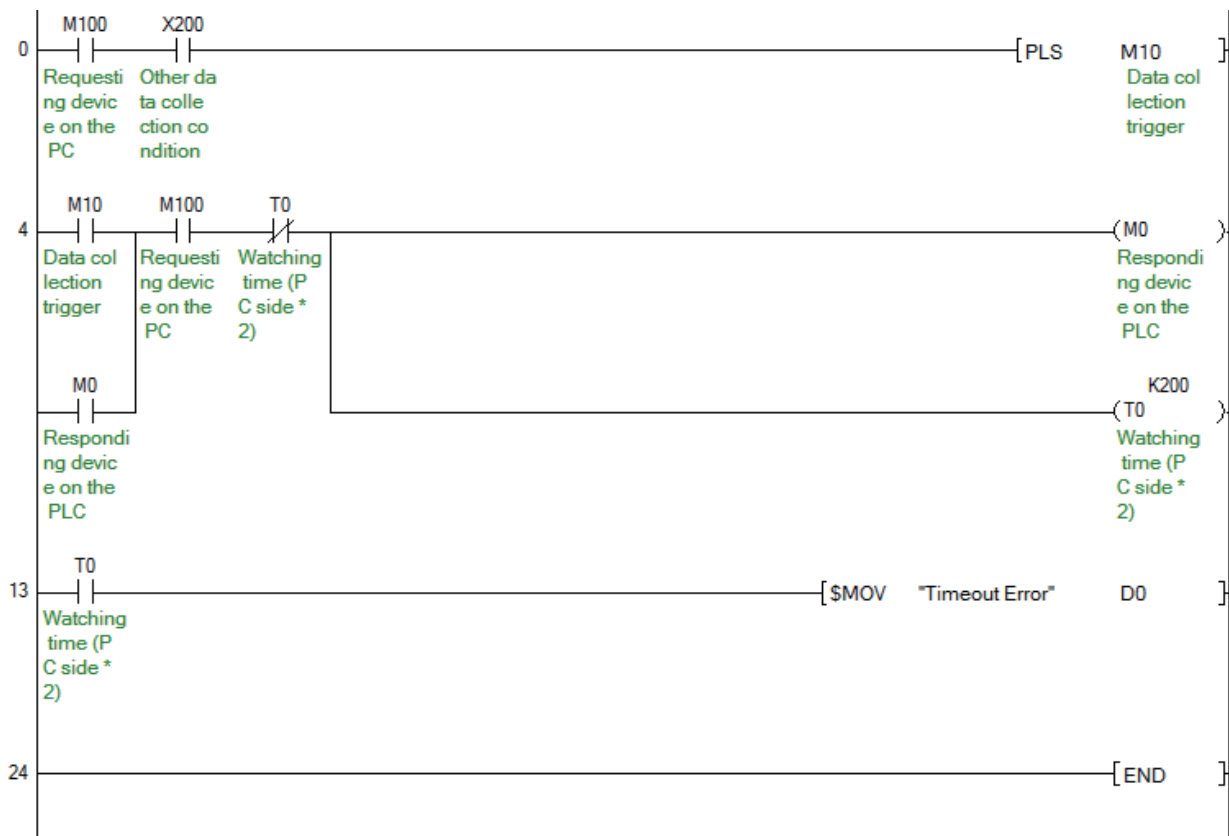

■When "Start with the request from the PC" is selected (Device: Word device)

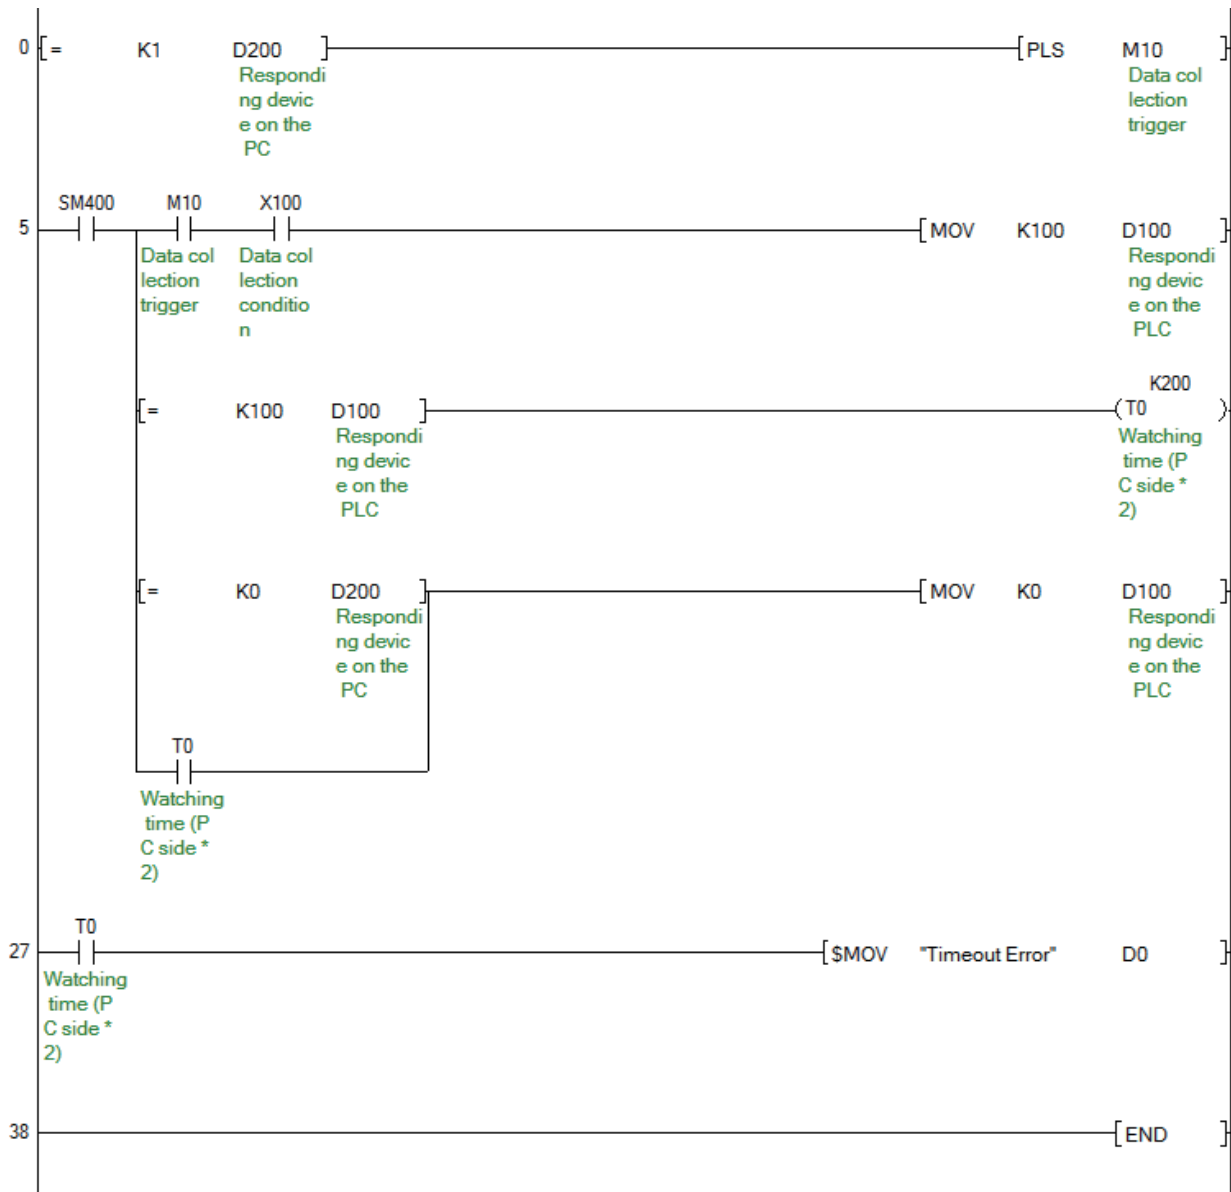


3

Setting of the [CSV Logging] tab

This section explains the setting of the [CSV Logging] tab for use of the logging function.

On the [CSV Logging] tab, the file name and the saving content with which logging data is saved to CSV file.

Window

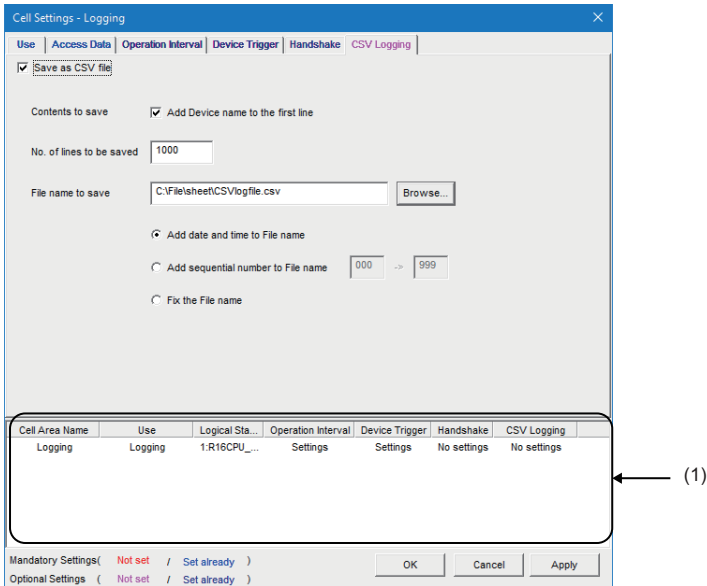

Displayed items

Item	Description	Reference
Save as CSV file	Set when using the CSV logging.	Page 81 "Save as CSV file"
Contents to save	Set when adding the device name to the first line.	Page 81 "Contents to save"
No. of lines to be saved	Set the number of lines to be saved.	Page 81 "No. of lines to be saved"
File name to save	Set the file name to save.	Page 82 "File name to save"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Save as CSV file"

Be sure to select the checkbox of "Save as CSV file" to use the CSV logging.

"Contents to save"

Activate this setting when adding the device name to the first line of the data to be saved into a CSV file.

Device name is added to first line.

```
DateTime,D0,D1,D2,D3,D4  
2021/04/23 15:57:09,25,16672,0,0,0  
2021/04/23 15:57:14,25,16672,0,0,0
```

If 0.001 to 0.999 seconds are set to the "Regular interval" on the [Operation Interval] tab, the date and time to be written to the CSV file is in the "yyyy/mm/dd hh:mm:ss" format.

Ex.

When 0.2 seconds interval is set

```
DateTime,D0,D1,D2  
2021/04/23 10:00,19,37,0,100  
2021/04/23 10:00,20,45,0,94  
2021/04/23 10:00,20,56,0,83  
2021/04/23 10:00,20,67,0,78  
2021/04/23 10:00,20,78,0,62  
2021/04/23 10:00,20,89,0,55  
2021/04/23 10:00,21,101,0,43
```



"No. of lines to be saved"

Set the number of lines to be saved into a single CSV file.

Setting range: 1 to 9999999

"File name to save"



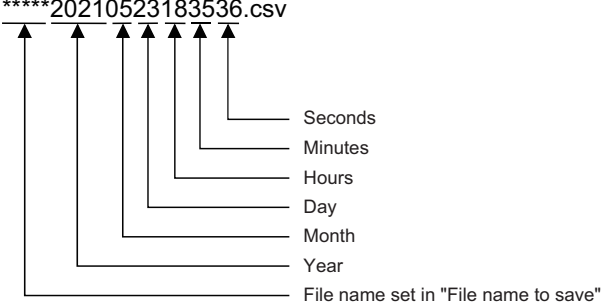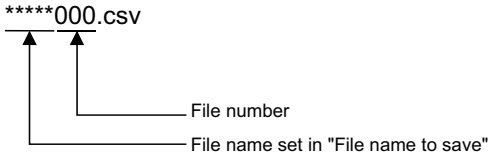



Set the CSV file name to save.

Item	Description
File name to save	Set the saving location and file name of the CSV file.*1
Add date and time to File name	<p>Adds the date and time data to the file name set in "File name to save" and saves it.</p> <p>In CSV logging, data is added until the data in the CSV file reach the number of lines set in "No. of lines to be saved". When they reach the set number of lines, a new CSV file is created.</p> <p>The following shows a file name format when data is saved.</p> <p>*****20210523183536.csv</p> 
Add sequential number to File name	<p>Adds the file number to the file name set in "File name to save" and saves it.</p> <p>A serial number can be set within the range from 000 to 999.</p> <p>When the number reaches to the last, the file of the first number is overwritten by the newly saving file.</p> <p>In CSV logging, data is added until the data in the CSV file reach the number of lines set in "No. of lines to be saved". When they reach the set number of lines, a new CSV file is created.</p> <p>The following shows a file name format when data is saved.</p> <p>*****000.csv</p> 
Fix the File name	<p>Overwrites data to the CSV file set in "File name to save".</p> <p>In CSV logging, data is added until the data in the CSV file reach the number of lines set in "No. of lines to be saved".</p>

*1 A UNC path name (\\server name\path name) cannot be specified as a file name. After assigning the network drive, specify the path name.

3.3 When "Monitor" is Selected


This section explains the "Cell Settings" screen when "Monitor" is selected from "Use" on the [Use] tab.

Tab	Required/optional	Reference
[Use] tab	Required setting	 Page 84 Setting of the [Use] tab
[Access Data] tab	Required setting	 Page 87 Setting of the [Access Data] tab
[Operation Interval] tab	Required setting	 Page 88 Setting of the [Operation Interval] tab
[Device Trigger] tab	Optional setting	 Page 89 Setting of the [Device Trigger] tab
[Handshake] tab	Optional setting	 Page 91 Setting of the [CSV Logging] tab
[CSV Logging] tab	Optional setting	 Page 90 Setting of the [Handshake] tab

Setting of the [Use] tab

This section explains the setting of the [Use] tab for use of the monitor function.
On the [Use] tab, set the cell area and monitor data display direction.

Window

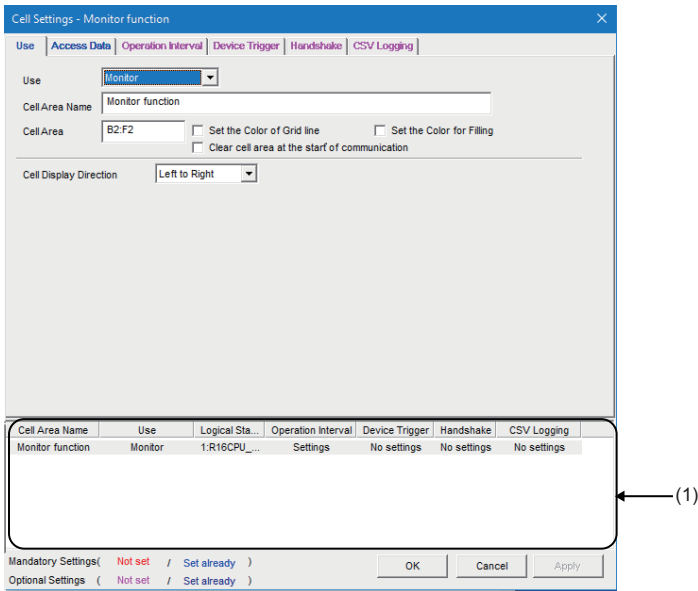

Displayed items

Item	Description	Reference
Use	Set the function to be used for the specified cell area. Select "Monitor" when using the monitor function.	—
Cell Area Name	Set the name of the specified cell area. (Maximum number of cell area names: 1000)	
Cell Area	Enter the value to specify the cell area.	Page 85 "Cell Area"
Set the Color of Grid line	Select this checkbox to add grid lines (including color designation) to the specified cell area.	Page 50 "Set the Color of Grid line" and "Set the Color for Filling"
Set the Color for Filling	Select this checkbox to color the specified cell area.	
Clear cell area at the start of communication	Select this checkbox to clear the data of specified cell area at the start of communication. (Default: cleared)	Page 85 "Clear cell area at the start of communication"
Cell Display Direction	Set the monitor data display sequence. <ul style="list-style-type: none"> • Left to Right Monitor data is displayed from left to right in the specified cell area in order. • Top to Bottom Monitor data is displayed from top to bottom in the specified cell area in order. 	Page 86 "Cell Display Direction"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Cell Area"

Set the cell area to be used by the monitor function.

■Setting examples

For the "Cell Area" setting examples, refer to the following:

☞ Page 49 "Cell Area"

■Setting ranges

The following shows the available number of cells and the number of specified cell areas.

Number of cells : 2000

Number of specified cell areas : 16

"Clear cell area at the start of communication"

Set whether or not to clear the data of cell area at the start of communication.

■Display example in the case where the checkbox of "Clear cell area at the start of communication" is selected

- Before the start of communication

1005	35	102	10
1002	30	200	15
990	36	151	25



- At the start of communication



- At the completion of the first collection

910	33	111	15
880	34	180	22
925	31	135	18

■Display example in the case where the checkbox of "Clear cell area at the start of communication" is not selected

- Before the start of communication

1005	35	102	10
1002	30	200	15
990	36	151	25



- At the start of communication

1005	35	102	10
1002	30	200	15
990	36	151	25



- At the completion of the first collection


910	33	111	15
880	34	180	22
925	31	135	18

"Cell Display Direction"

Set the monitor data display sequence.

■When "Left to Right" is selected

- Cell area (B2:D5)

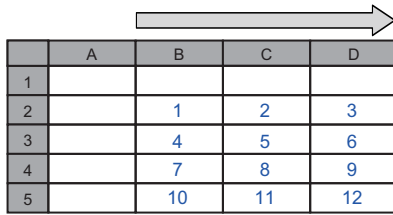


	A	B	C	D
1				
2		1	2	3
3		4	5	6
4		7	8	9
5		10	11	12

Monitor data are displayed in order of 1 to 12.

■When "Top to Bottom" is selected

- Cell area (B2:D5)

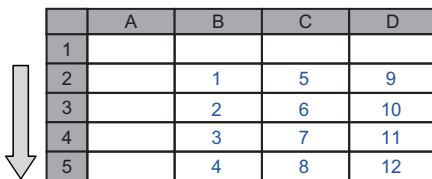

	A	B	C	D
1				
2		1	5	9
3		2	6	10
4		3	7	11
5		4	8	12


Monitor data are displayed in order of 1 to 12.

Setting of the [Access Data] tab

This section explains the setting of the [Access Data] tab for use of the monitor function.

On the [Access Data] tab, set the logical station number required for communication with a CPU module and the device data to be collected in the cell area.

Window

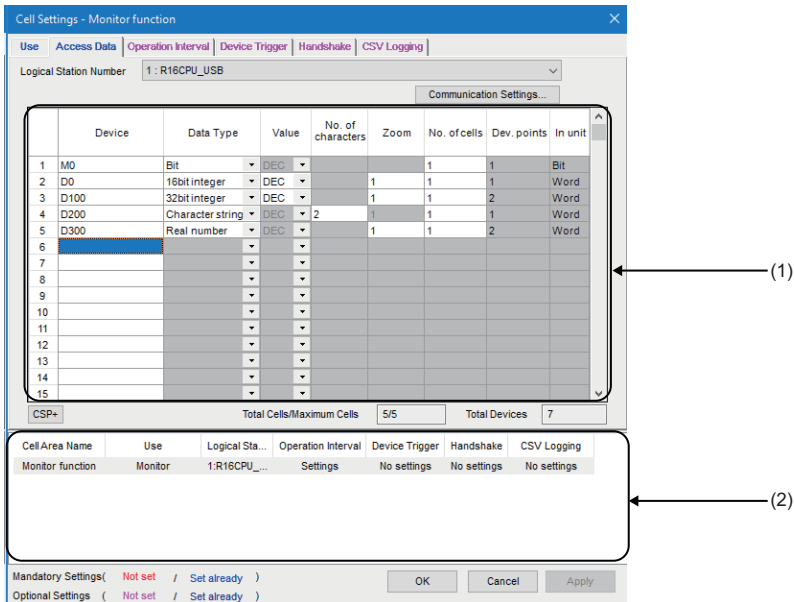

Displayed items


Item	Description	Reference
Logical Station Number	Select the logical station number required for communication.	Page 55 "Logical Station Number"
[Communication Settings] button	Click this to start Communication Settings Utility for setting a new logical station number and changing settings.	Page 56 [Communication Settings] button
Remote password* ¹	Enter the password when the password is set to the connection target CPU module.	Page 56 "Remote password"
(1) (Access data)	Set the devices or labels to be monitored.	Page 56 Access data
[CSP+] button	Click this to display the "Getting CSP+ for machine" screen.	Page 60 Importing CSP+ for machine
Total Cells/Maximum Cells	The number of cells for which a device is set in a cell area/the number of cells that can be set in the area is displayed.	—
Total Devices	The number of device points set in the cell area is displayed.	—
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

*1 "Remote password" is displayed when the logical station number selected in "Logical Station Number" on the [Access Data] tab is the one for the password function compatible module.

Setting of the [Operation Interval] tab

This section explains the setting of the [Operation Interval] tab for use of the monitor function.
 On the [Operation Interval] tab, set the day and time of the activation of the function for the cell area.

Window

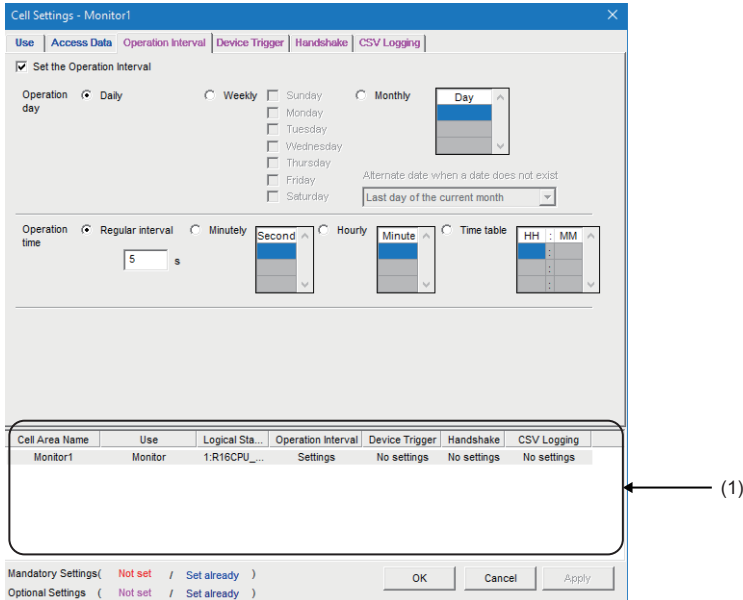

Displayed items

Item	Description	Reference
Set the Operation Interval	Set the operation of the cell area valid or invalid.	Page 62 "Set the Operation Interval"
Operation day	Set the operation day of the monitor function activation.	Page 62 "Operation day"
Operation time	Set the operation time of the monitor function activation.	Page 88 "Operation time"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Operation time"

The setting except for "Regular interval" is the same as that of the logging function.

☞ Page 63 "Operation time"

■When "Regular interval" is selected

Device data is collected at the set second intervals.

When setting lesser "seconds" than the actual communication time, the fixed interval communication cannot be established.

Hence, set for longer than the actual communication time.

For Communication time, refer to the following performance value.


☞ Page 161 Processing Speed of MX Sheet

Setting range: 0.001 to 0.999 (in units of 0.001 seconds), 1 to 3600 (in units of 1 second)

Setting of the [Device Trigger] tab

This section explains the setting of the [Device Trigger] tab for use of the monitor function.
 On the [Device Trigger] tab, set the device conditions for the device trigger.

Window

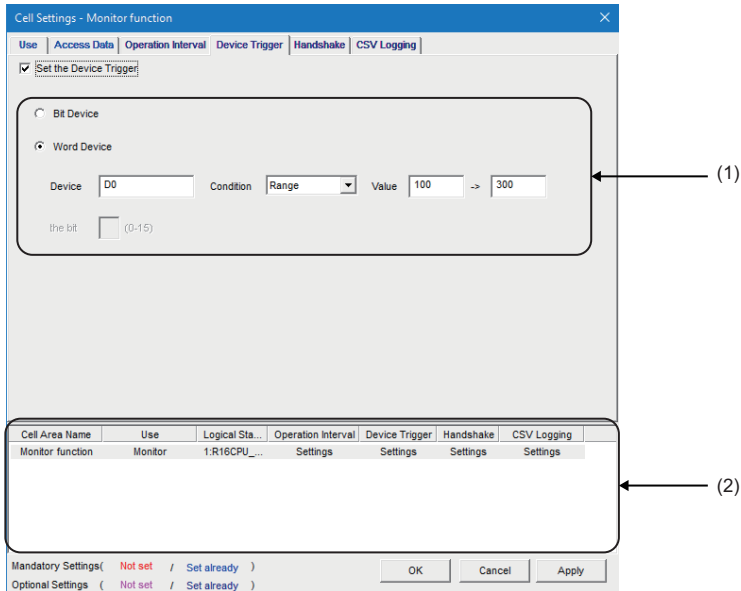


Displayed items

Item	Description	Reference
Set the Device Trigger	Set when the device trigger is used.	Page 67 "Set the Device Trigger"
(1) (Device conditions)	Set the device or label conditions.	Page 67 Device conditions
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Setting of the [Handshake] tab

This section explains the setting of the [Handshake] tab for use of the monitor function. On the [Handshake] tab, set the handshake requesting source and handshake processing.

Window

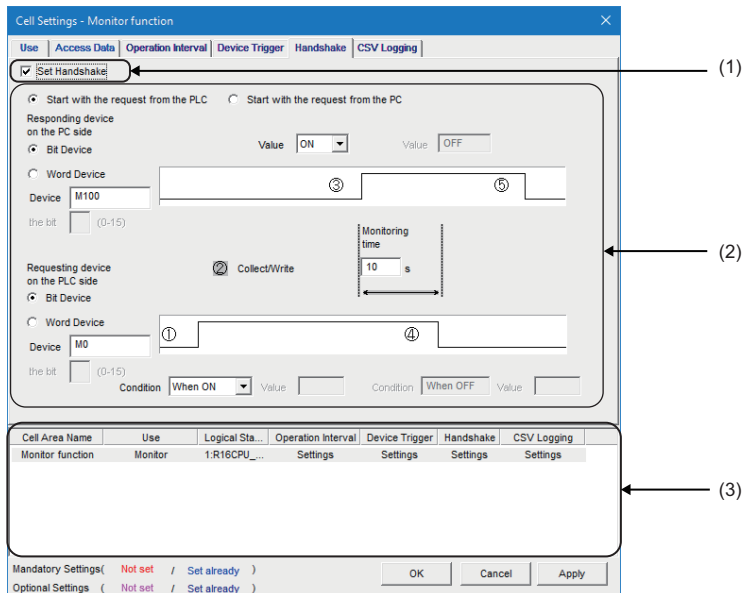

Displayed items


Item	Description	Reference
Set Handshake	Set when using a handshake.	Page 74 "Set Handshake"
(1) (Requesting source setting)	Set the requesting source of the handshake.	Page 74 Requesting source setting
(2) (Handshake processing)	Set the handshake processing.	Page 74 Handshake processing
(3) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Setting of the [CSV Logging] tab

This section explains the setting of the [CSV Logging] tab for use of the monitor function.

On the [CSV Logging] tab, set the file name and the saving content with which the monitor data is saved into the CSV file.

Window

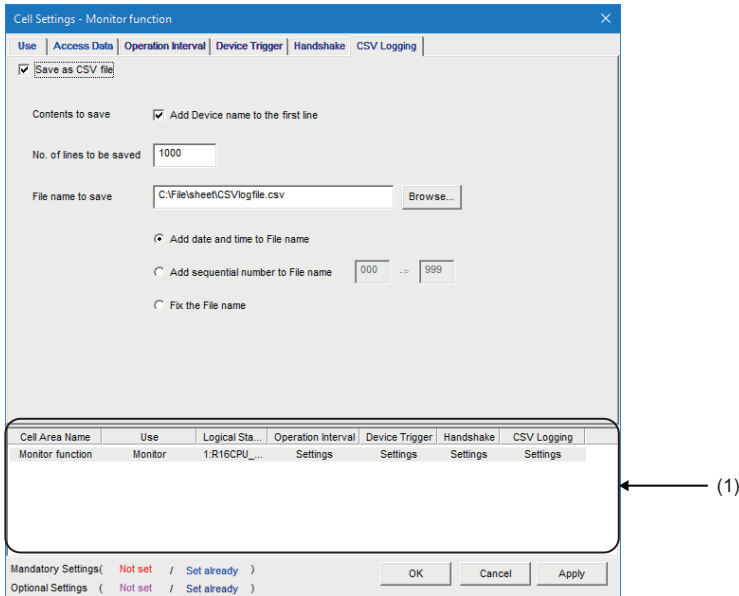






Displayed items

Item	Description	Reference
Save as CSV file	Set when using the CSV logging.	Page 81 "Save as CSV file"
Contents to save	Set when adding the device name to the first line.	Page 81 "Contents to save"
No. of lines to be saved	Set the number of lines to be saved.	Page 81 "No. of lines to be saved"
File name to save	Set the file name to save.	Page 82 "File name to save"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

3.4 When "Write" is Selected


This section explains the "Cell Settings" screen when "Write" is selected from "Use" on the [Use] tab.

Tab	Required/optional	Reference
[Use] tab	Required setting	 Page 93 Setting of the [Use] tab
[Access Data] tab	Required setting	 Page 95 Setting of the [Access Data] tab
[Operation Interval] tab	Required setting	 Page 97 Setting of the [Operation Interval] tab
[Device Trigger] tab	Optional setting	 Page 98 Setting of the [Device Trigger] tab
[Handshake] tab	Optional setting	 Page 99 Setting of the [Handshake] tab

Setting of the [Use] tab

This section explains the setting of the [Use] tab for use of the write function. On the [Use] tab, set the cell area and display direction of write data.

Window

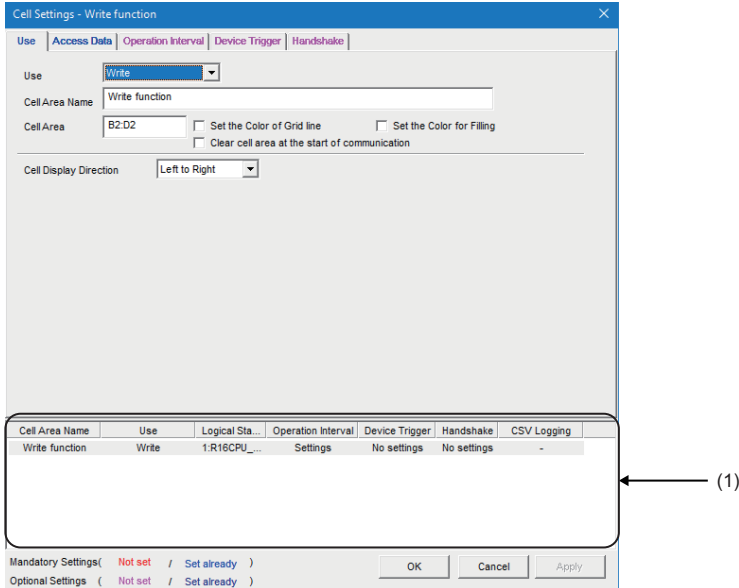

Displayed items

Item	Description	Reference
Use	Set the function to be used for the specified cell area. Select "Write" when using the write function.	—
Cell Area Name	Set the name of the specified cell area. (Maximum number of cell area names: 1000)	
Cell Area	Enter the value to specify the cell area.	Page 94 "Cell Area"
Set the Color of Grid line	Select this checkbox to add grid lines (including color designation) to the specified cell area.	Page 50 "Set the Color of Grid line" and "Set the Color for Filling"
Set the Color for Filling	Select this checkbox to color the specified cell area.	
Clear cell area at the start of communication	Select this checkbox to clear the data of specified cell area at the start of communication. (Default: cleared)	Page 85 "Clear cell area at the start of communication"
Cell Display Direction	Set the display sequence of write data. <ul style="list-style-type: none"> • Left to Right Write data is set from left to right in the specified cell area in order. • Top to Bottom Write data is set from top to bottom in the specified cell area in order. 	Page 94 "Cell Display Direction"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Cell Area"

Set the cell area to be used by the write function.

■Setting examples

For the "Cell Area" setting examples, refer to the following:

☞ Page 49 "Cell Area"

■Setting ranges

The following shows the available number of cells and the number of specified cell areas.

Number of cells : 2000


Number of specified cell areas : 16

"Cell Display Direction"

Set the display sequence of write data.

■When "Left to Right" is selected

- Cell area (B2:D5)

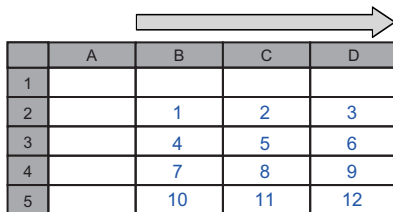


	A	B	C	D
1				
2		1	2	3
3		4	5	6
4		7	8	9
5		10	11	12

Monitor data are displayed in order of 1 to 12.

■When "Top to Bottom" is selected

- Cell area (B2:D5)

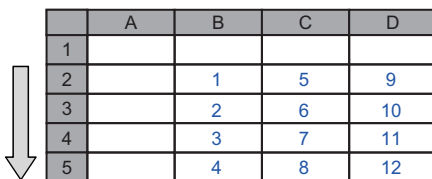

	A	B	C	D
1				
2		1	5	9
3		2	6	10
4		3	7	11
5		4	8	12


Monitor data are displayed in order of 1 to 12.

Setting of the [Access Data] tab

This section explains the setting of the [Access Data] tab for use of the write function.

On the [Access Data] tab, set the logical station number required for communication with a CPU module and the device data to be written from the cell area.

Window

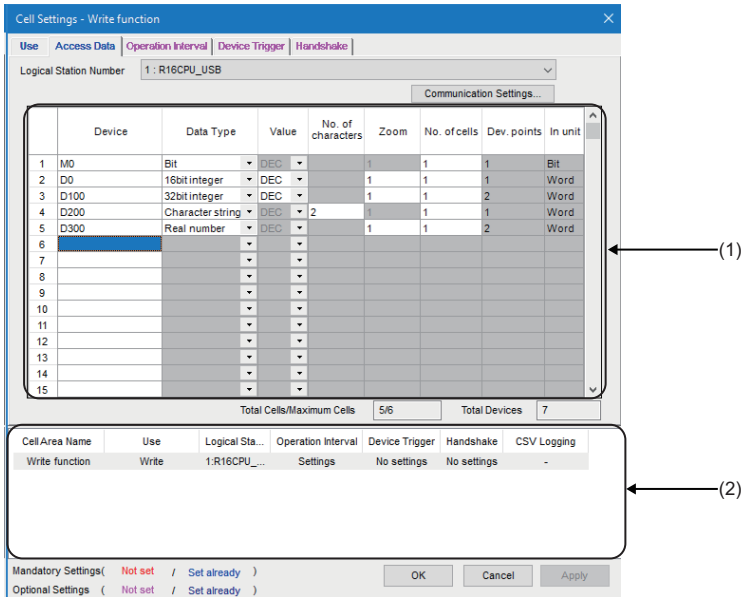

Displayed items

Item	Description	Reference
Logical Station Number	Select the logical station number required for communication.	Page 55 "Logical Station Number"
[Communication Settings] button	Click this to start Communication Settings Utility for setting a new logical station number and changing settings.	Page 56 [Communication Settings] button
Remote password*1	Enter the password when the password is set to the connection target CPU module.	Page 56 "Remote password"
(1) (Access data)	Set the devices or labels to be written.	Page 96 Access data
Total Cells/Maximum Cells	The number of cells for which a device is set in a cell area/the number of cells that can be set in the area is displayed.	—
Total Devices	The number of device points set in the cell area is displayed.	—
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

*1 "Remote password" is displayed when the logical station number selected in "Logical Station Number" on the [Access Data] tab is the one for the password function compatible module.

Access data

The setting except for "Zoom" is the same as that of the logging function.


☞ Page 55 Setting of the [Access Data] tab

■ "Zoom"

The value entered into the cell is multiplied by the zoom ratio and written to a CPU module device.

When "Data Type" is set to "Bit" or "Character string" or when "Value" is set to "HEX", "Zoom" cannot be set.

Setting range: 0.001 to 1000

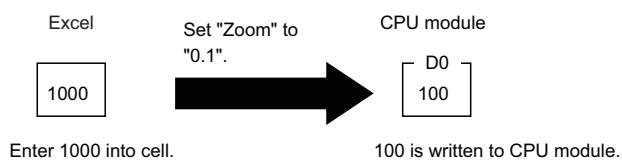


Point

When "Zoom" is set for the write data and the data to be actually written to a CPU module is decimals, set "Real number" in "Data type."

Setting of the [Operation Interval] tab

This section explains the setting of the [Operation Interval] tab for use of the write function.
 On the [Operation Interval] tab, set the day and time of the activation of the function for the cell area.

Window

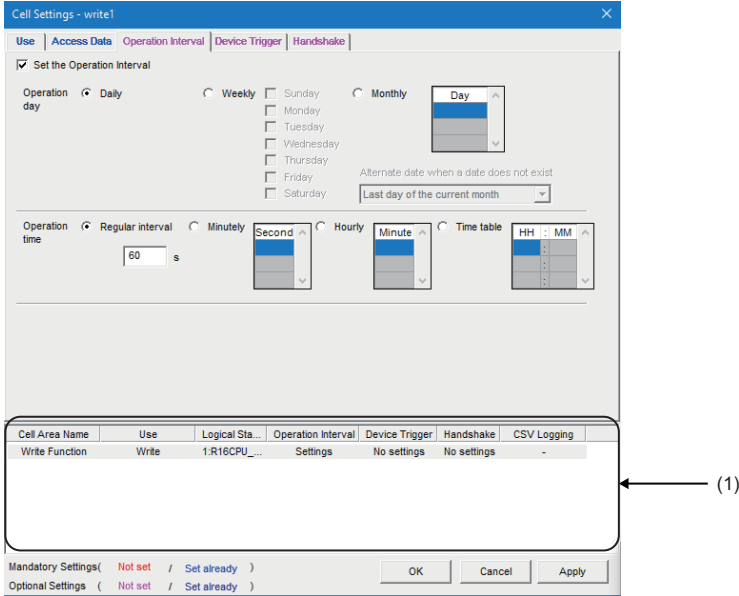

Displayed items

Item	Description	Reference
Set the Operation Interval	Set the operation of the cell area valid or invalid.	Page 62 "Set the Operation Interval"
Operation day	Set the operation day of the write function activation.	Page 62 "Operation day"
Operation time	Set the operation time of the write function activation.	Page 97 "Operation time"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Operation time"

The setting except for "Regular interval" is the same as that of the logging function.

☞ Page 63 "Operation time"

■When "Regular interval" is selected

Device data is written at the set second intervals.

When setting lesser "seconds" than the actual communication time, the fixed interval communication cannot be established.

Hence, set for longer than the actual communication time.

For Communication time, refer to the following performance value.


☞ Page 161 Processing Speed of MX Sheet

Setting range: 0.001 to 0.999 (in units of 0.001 seconds), 1 to 3600 (in units of 1 second)

Setting of the [Device Trigger] tab

This section explains the setting of the [Device Trigger] tab for use of the write function.
 On the [Device Trigger] tab, set the device conditions for the device trigger.

Window

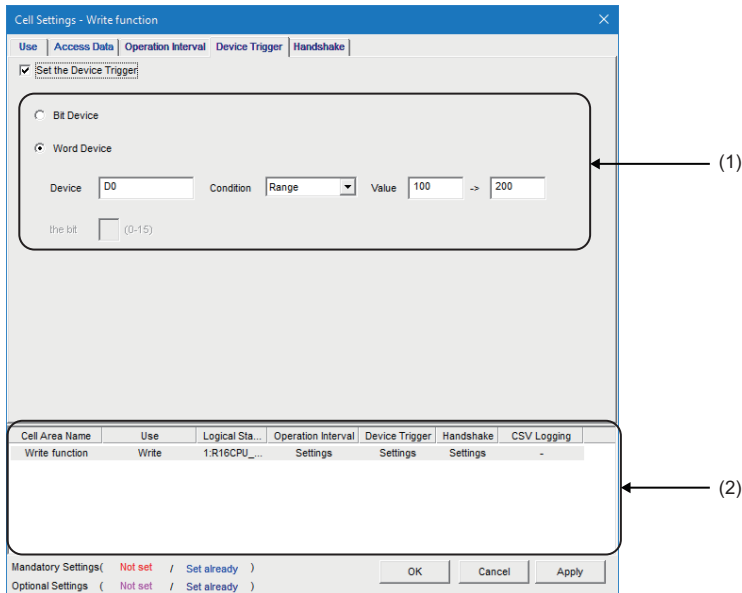


Displayed items

Item	Description	Reference
Set the Device Trigger	Set when the device trigger is used.	Page 67 "Set the Device Trigger"
(1) (Device conditions)	Set the device or label conditions.	Page 67 Device conditions
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Setting of the [Handshake] tab

This section explains the setting of the [Handshake] tab for use of the write function. On the [Handshake] tab, set the handshake requesting source and handshake processing.

Window

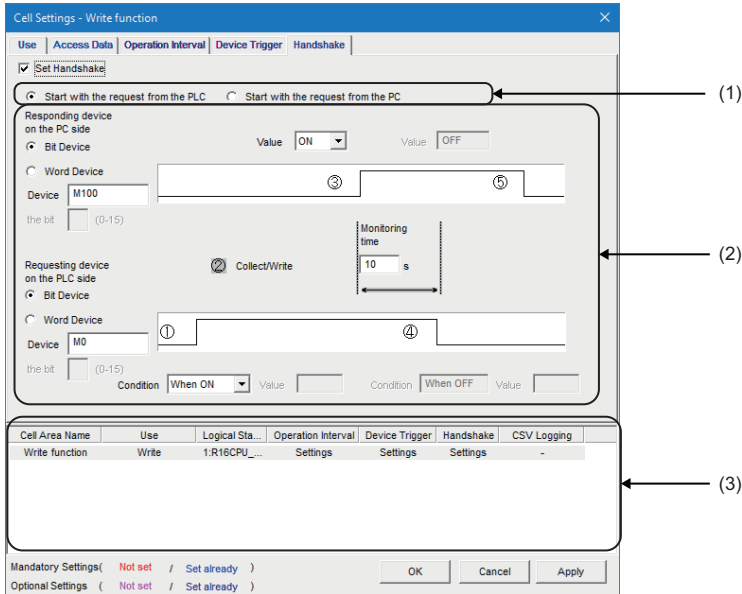






Displayed items

Item	Description	Reference
Set Handshake	Set when using a handshake.	Page 74 "Set Handshake"
(1) (Requesting source setting)	Set the requesting source of the handshake.	Page 74 Requesting source setting
(2) (Handshake processing)	Set the handshake processing.	Page 74 Handshake processing
(3) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

3.5 When "Alarm Summary" is Selected

This section explains the "Cell Settings" screen when "Alarm summary" is selected from "Use" on the [Use] tab.


Tab	Required/optional	Reference
[Use] tab	Required setting	 Page 101 Setting of the [Use] tab
[Access Data] tab	Required setting	 Page 104 Setting of the [Access Data] tab
[Alarm Data] tab	Optional setting	 Page 106 Setting of the [Alarm Data] tab
[Operation Interval] tab	Optional setting	 Page 108 Setting of the [Operation Interval] tab
[Device Trigger] tab	Optional setting	 Page 109 Setting of the [Device Trigger] tab

Setting of the [Use] tab

This section explains the setting of the [Use] tab for use of the alarm summary function.

On the [Use] tab, set the cell area, display position of alarm data and operation in the case where cell is full.

Window

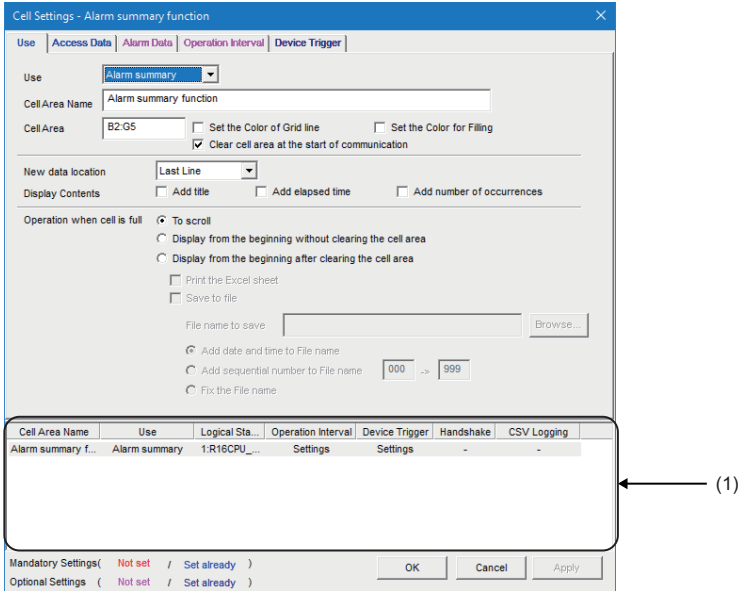

Displayed items

Item	Description	Reference
Use	Set the function to be used for the specified cell area. Select "Alarm summary" when using the alarm summary function.	—
Cell Area Name	Set the name of the specified cell area. (Maximum number of cell area names: 100)	
Cell Area	Enter the value to specify the cell area.	Page 102 "Cell Area"
Set the Color of Grid line	Select this checkbox to add grid lines (including color designation) to the specified cell area.	Page 50 "Set the Color of Grid line" and "Set the Color for Filling"
Set the Color for Filling	Select this checkbox to color the specified cell area.	
Clear cell area at the start of communication	Select this checkbox to clear the data of specified cell area at the start of communication. (Default: selected)	Page 50 "Clear cell area at the start of communication"
New data location	Set the latest data display position of the alarm summary. • Last Line The latest data is displayed at the last of the specified cell area. • First Line The latest data is displayed at the first of the specified cell area.	Page 51 "New data location"
Display Contents	Set whether the title, elapsed time, and number of occurrences is added to the Alarm Summary or not.	Page 102 "Display Contents"
Operation when cell is full	Set the operation to be performed when the specified cell area is full. • To scroll The displayed contents are scrolled and displayed. • Display from the beginning without clearing the cell area The data currently displayed in the cell area are overwritten and the alarm summary is resumed. Before the alarm summary is resumed, the Excel spreadsheet can be printed and saved. • Display from the beginning after clearing the cell area The data displayed in the cell area are erased and the alarm summary is resumed. Before the alarm summary is resumed, the Excel spreadsheet can be printed and saved.	Page 53 "Operation when cell is full"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Cell Area"

Set the cell area to be used by the alarm summary function.

■Setting examples

For the "Cell Area" setting examples, refer to the following:

☞ Page 49 "Cell Area"

■Setting ranges

The following shows the available number of cells and the number of specified cell areas.

Number of cells : 4 columns (indispensable) × 65536 rows *1

Number of specified cell areas : 16

*1 When displaying the elapsed time and number of occurrences in the Alarm Summary, increase the number of columns by 1 respectively. 6 columns are required to display both.

"Display Contents"

■"Add title" checkbox

Set whether the title for the column item shown in the following table is displayed or not on the first line of the set "Cell Area". Select this check box to display the title.

Column item	Title
ON time String/OFF time String(☞ Page 106 Setting of the [Alarm Data] tab) "ON time String" is displayed when the device turns from OFF to ON. "OFF time String" is displayed when the device turns from ON to OFF.	ON/OFF
Date and time when the device turns from OFF to ON or from ON to OFF	Date time
Alarm String set to the device(☞ Page 106 Setting of the [Alarm Data] tab)	Alarm
Status String set to the device(☞ Page 106 Setting of the [Alarm Data] tab)	Status
Elapsed time from when the device turns ON until it turns OFF(☞ Page 102 "Add elapsed time" checkbox)	Elapsed time
Number of times when the device turned from OFF to ON after the start of communication.(☞ Page 103 "Add number of occurrences" checkbox)	Number of occurrences

Point

- The title display line is not the target of cell area clear at the start of communication or clear when cell is full.
- When the Cell Area is set at multiple locations, the title is displayed for only the Cell Area specified first.

■"Add elapsed time" checkbox

Set whether the elapsed time from when the device set on the [Access Data] tab turns ON until it turns OFF is displayed on the Alarm Summary or not.

Select this checkbox to display the elapsed time.

The display format is "hour:minute:second".

Ex.

Display when the elapsed time is 1 minute 25 seconds

0:01:25

Point

When the device is ON at the start of communication, the time from when communication starts until the device turns OFF is displayed as the elapsed time.

■ "Add number of occurrences" checkbox

Set whether the number of times when the device set on the [Access Data] tab turns from OFF to ON after the start of communication is displayed on the Alarm Summary or not.

Select this check box to display the number of occurrences.

In this case, the "Clear cell area at the start of communication" checkbox must be selected.

Point

- When the device is ON at the start of communication, it is counted as the first alarm.
- When the number of occurrences exceeds 65535, it returns to 0.

Ex.

Display content on the Excel spreadsheet when the checkboxes of "Add title", "Add elapsed time", and "Add number of occurrences" are all selected


ON/OFF	Date time	Alarm	Status	Elapsed time	Number of occurrences
Generation	2012/05/24 Thu 15:05:20	Parts1 Abnormal fault	Major failure	(Blank)	1
Generation	2012/05/24 Thu 15:05:31	Parts 2 Quantity error	Minor failure	(Blank)	1
Restoration	2012/05/24 Thu 15:06:48	Parts1 Abnormal fault	Major failure	0:01:28	1
Restoration	2012/05/24 Thu 15:07:52	Parts 2 Quantity error	Minor failure	0:02:21	1

Setting of the [Access Data] tab

This section explains the setting of the [Access Data] tab for use of the alarm summary function.

On the [Access Data] tab, set the logical station number required for communication with a CPU module and the device data to be used for the alarm summary function.

Window

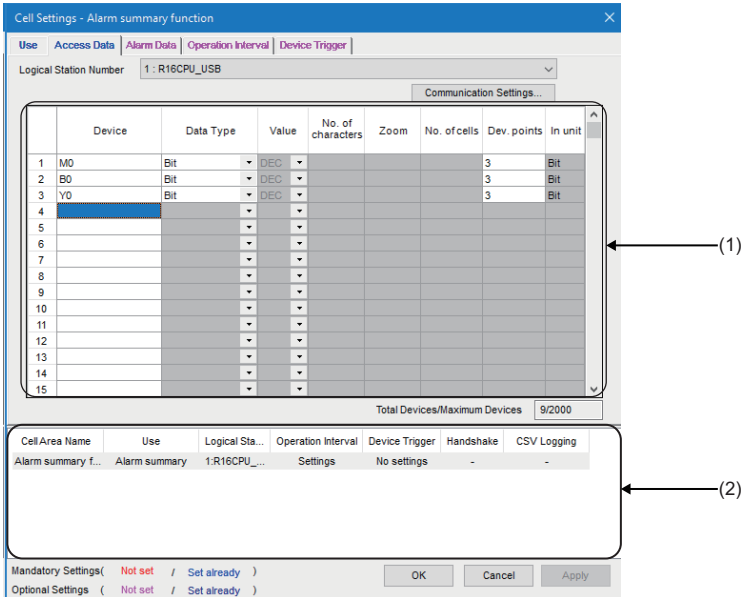

Displayed items

Item	Description	Reference
Logical Station Number	Select the logical station number required for communication.	Page 55 "Logical Station Number"
[Communication Settings] button	Click this to start Communication Settings Utility for setting a new logical station number and changing settings.	Page 56 [Communication Settings] button
Remote password*1	Enter the password when the password is set to the connection target CPU module.	Page 56 "Remote password"
(1) (Access data)	Set the devices or labels use for the alarm summary function.	Page 105 Access data
Total Devices/Maximum Devices	The number of devices that are registered/devices that can be registered in the cell area is displayed.	—
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

*1 "Remote password" is displayed when the logical station number selected in "Logical Station Number" on the [Access Data] tab is the one for the password function compatible module.

Access data

Registration order

Data is displayed on the [Alarm Data] tab in the order of the numbers shown on the left of the [Access Data] tab.

Setting example of [Access Data] tab

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	M0	Bit	DEC				3	Bit
2	B0	Bit	DEC				3	Bit
3	Y0	Bit	DEC				3	Bit

Data numbers

The device data is displayed on the [Alarm Data] tab as shown below.

	Device	ON time String
Data No. 1	1 M0	Generation
	2 M1	Generation
	3 M2	Generation
Data No. 2	4 B0	Generation
	5 B1	Generation
	6 B2	Generation
Data No. 3	7 Y0	Generation
	8 Y1	Generation
	9 Y2	Generation

Displayed in order of data numbers.

"Device"

Only the bit device can be specified for the alarm summary.

Enter a device name and device number in this order.


"Dev. Points"

The points of the devices to be consecutively registered starting with the device number set in "Device" are displayed.

Setting of the [Alarm Data] tab

This section explains the setting of the [Alarm Data] tab for use of the alarm summary function. On the [Alarm Data] tab, set the character strings to be displayed in the cell area.

Window

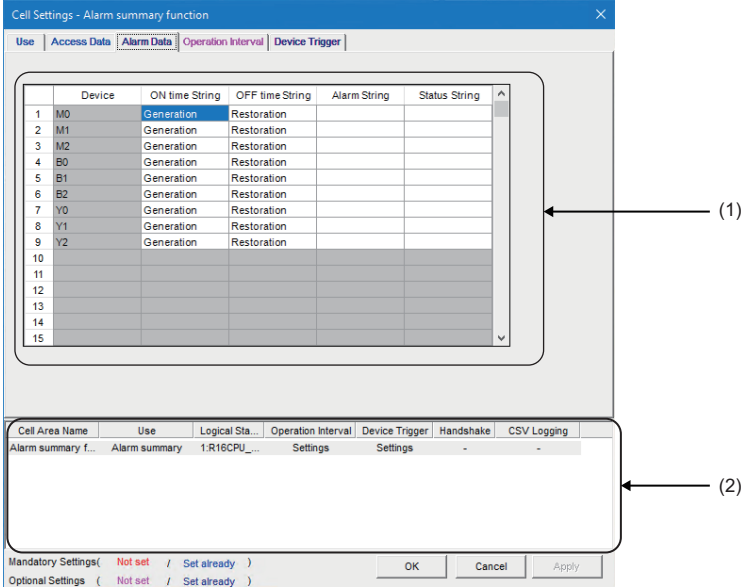

Displayed items

Item	Description	Reference
(1) (Alarm data)	Set the alarm data to be used for the alarm summary function.	Page 106 "Device" to Page 107 "Status String"
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Device"

The device or label registered on the [Access Data] tab is displayed.

"ON time String"

Enter the character string to be displayed in the cell when the registered device turns ON.

Number of characters: Up to 16

"OFF time String"

Enter the character string to be displayed in the cell when the registered device turns OFF.

Number of characters: Up to 16

"Alarm String"

Enter an alarm character string.

Number of characters: Up to 40

"Status String"

Enter a status character string.

Number of characters: Up to 16

Setting examples

The following shows the [Alarm Data] tab setting example and the data displayed on the Excel spreadsheet.

- [Alarm Data] tab setting example

	Device	ON time String	OFF time String	Alarm String	Status String
1	M0	Generation	Restoration	Material shortage	Minor failure
2					

Item	Setting
Device	M0
ON time String	Generation
OFF time String	Restoration
Alarm String	Material shortage
Status String	Minor failure

- Operation of M0



- Data displayed on Excel spreadsheet

Displayed in order of "date and time of occurrence", "alarm character string" and "status character string".


Displayed in the cell when M0 is ON (1).

Displayed in the cell when M0 is OFF (2).

Setting of the [Operation Interval] tab

This section explains the setting of the [Operation Interval] tab for use of the alarm summary function. On the [Operation Interval] tab, set the operation interval for the function of the cell area.

Window

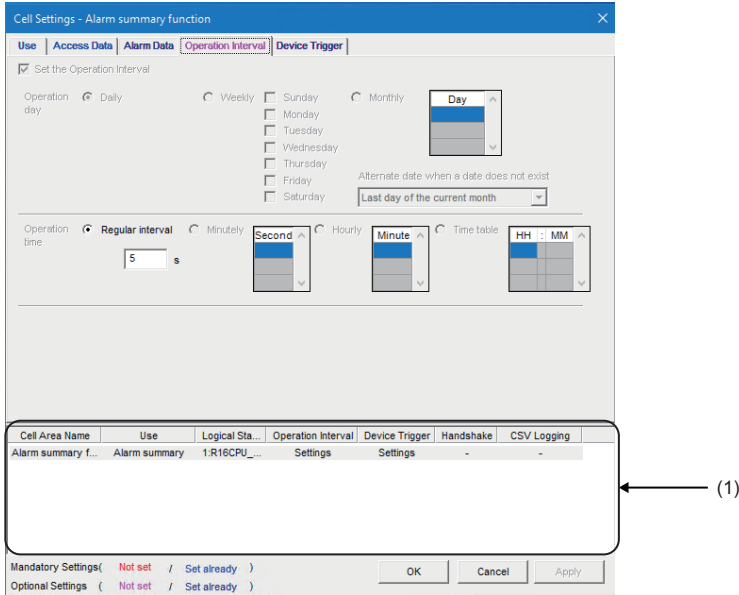

Displayed items

Item	Description	Reference
Regular interval	Set the operation interval of the alarm summary function.	Page 108 "Regular interval"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Regular interval"


Device data is collected at the set second intervals.

Setting range: 0.001 to 0.999 (in units of 0.001 seconds), 1 to 3600 (in units of 1 second)

If 0.001 to 0.999 seconds are set to the "Regular interval" on the [Operation Interval] tab, the ON/OFF time displayed on the Excel spreadsheet is in the "yyyy/mm/dd ddd hh:mm:ss" format.

Ex.


When 0.2 seconds interval is set and the ON time is 20 hours 41 minutes 12 seconds 80

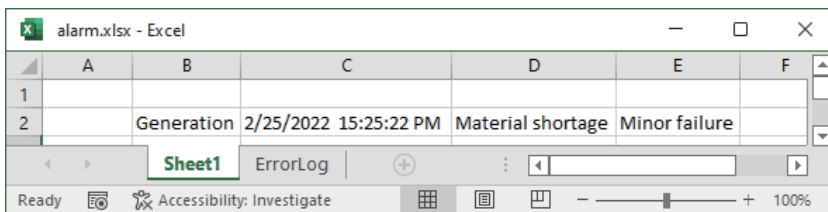

Setting of the [Device Trigger] tab

This section explains the setting of the [Device Trigger] tab for use of the alarm summary function. On the [Device Trigger] tab, set the device conditions for the device trigger.

Window

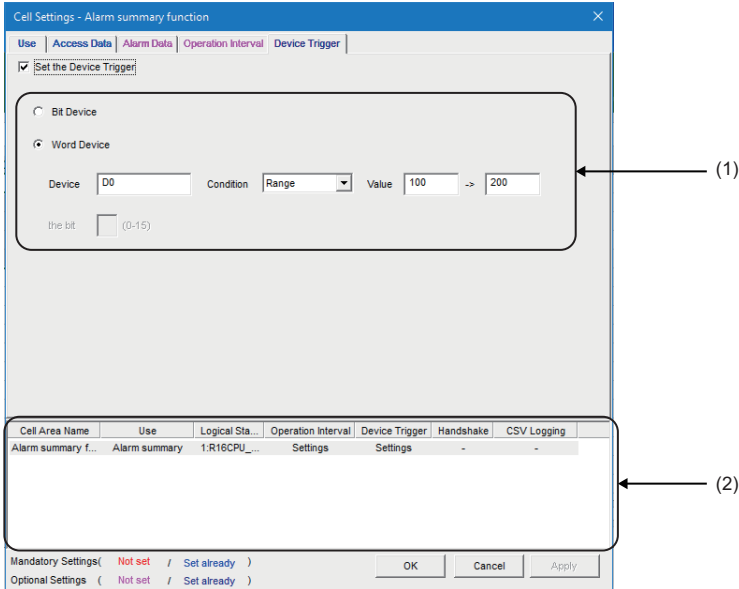

Displayed items

Item	Description	Reference
Set the Device Trigger	Set when the device trigger is used.	Page 67 "Set the Device Trigger"
(1) (Device conditions)	Set the device or label conditions.	Page 67 Device conditions
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

3.6 When "Comment" is Selected


This section explains the "Cell Settings" screen when "Comment" is selected from "Use" on the [Use] tab.

Tab	Required/optional	Reference
[Use] tab	Required setting	☞ Page 111 Setting of the [Use] tab
[Access Data] tab	Required setting	☞ Page 112 Setting of the [Access Data] tab
[Comment Data] tab	Required setting	☞ Page 114 Setting of the [Comment Data] tab
[Operation Interval] tab	Optional setting	☞ Page 116 Setting of the [Operation Interval] tab
[Device Trigger] tab	Optional setting	☞ Page 117 Setting of the [Device Trigger] tab
[Handshake] tab	Optional setting	☞ Page 118 Setting of the [Handshake] tab

Setting of the [Use] tab

This section explains the setting of the [Use] tab for use of the comment display function.
On the [Use] tab, set the cell area.

Window

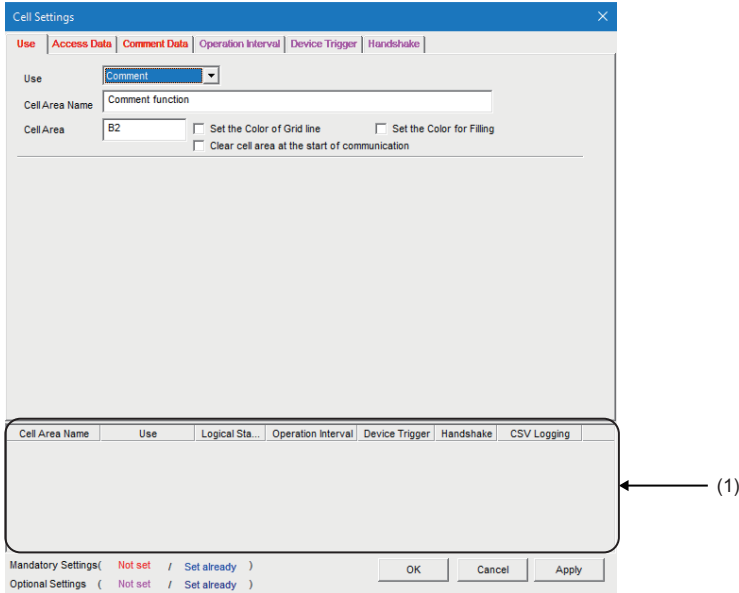

Displayed items


Item	Description	Reference
Use	Set the function to be used for the specified cell area. Select "Comment" when using the comment display function.	—
Cell Area Name	Set the name of the specified cell area. (Maximum number of cell area names: 500)	—
Cell Area	Set the cell area to be used by the comment display function. Setting range: 1	—
Set the Color of Grid line	Select this checkbox to add grid lines (including color designation) to the specified cell area.	Page 50 "Set the Color of Grid line" and "Set the Color for Filling"
Set the Color for Filling	Select this checkbox to color the specified cell area.	
Clear cell area at the start of communication	Select this checkbox to clear the data of specified cell area at the start of communication. (Default: cleared)	Page 50 "Clear cell area at the start of communication"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Setting of the [Access Data] tab

This section explains the setting of the [Access Data] tab for use of the comment display function.

On the [Access Data] tab, set the logical station number required for communication with a CPU module and the device data to be used for the comment display function.

Window

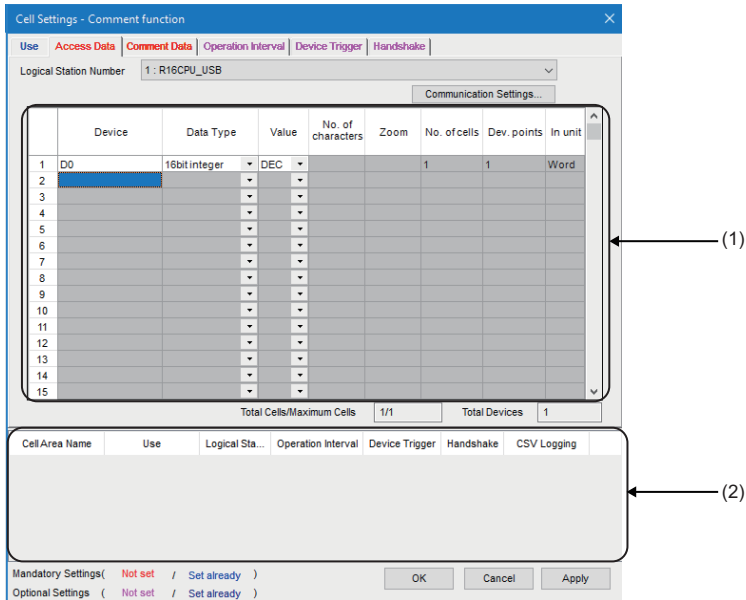

Displayed items

Item	Description	Reference
Logical Station Number	Select the logical station number required for communication.	Page 55 "Logical Station Number"
[Communication Settings] button	Click this to start Communication Settings Utility for setting a new logical station number and changing settings.	Page 56 [Communication Settings] button
Remote password*1	Enter the password when the password is set to the connection target CPU module.	Page 56 "Remote password"
(1) (Access data)	Set a device or label used for the comment display function.	Page 113 Access data
Total Cells/Maximum Cells	The number of cells for which a device is set in a cell area/the number of cells that can be set in the area is displayed.	—
Total Devices	The number of device points set in the cell area is displayed.	—
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

*1 "Remote password" is displayed when the logical station number selected in "Logical Station Number" on the [Access Data] tab is the one for the password function compatible module.

Access data

■ "Device"

Set a device or label used for the comment display function.

- When entering a device, enter in the order of a device name and device number.
- When entering a label, enter the label name.
- The applicable data types are Bit and Word.
- When entering a label, enter other than structured data type label and array type label.

For the accessible devices, refer to the following:

 Page 19 Accessible range

■ "Data Type"


Set the data type of the device used for the comment display function.

Item	Available Device	Description
Bit	Bit device	Set when bit devices set in "Device" are used for the comment display function.
	Word device (Bit specification)	Set when designated bits for word devices set in "Device" are used for the comment display function (e.g. D0.0).
16 bit integer (-32768 to 32767)	Bit device	Set when 1 word (16 bits), starting from the device number set in 16 bit integer "Device", is used for the comment display function.
	Word device	Set when the word device set in "Device" is used for the comment display function.
32 bit integer (-2147483648 to 2147483647)	Bit device	Set when 2 words (32 bits), starting from the device number set in "Device", are used for the comment display function.
	Word device	Set when 2 words, starting from the device number set in "Device", are used for the comment display function.
	Double word device	Set when double word devices set in "Device" are used for the comment display function.

Setting of the [Comment Data] tab

This section explains the setting of the [Comment Data] tab for use of the comment display function. On the [Comment Data] tab, set the comment data to be displayed in the cell area.

Window

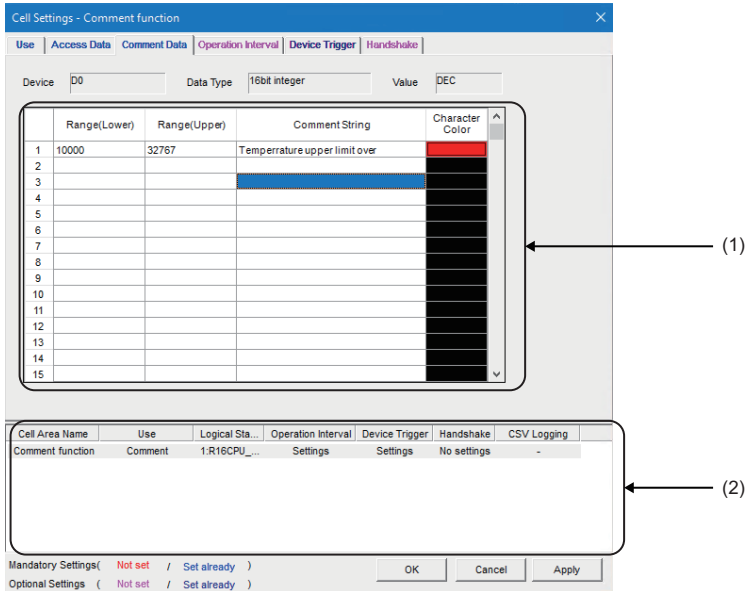

Displayed items

Item	Description	Reference
Device	The device set in "Device" on the [Access Data] tab is displayed.	—
Data Type	The data type set in "Data Type" on the [Access Data] tab is displayed.	
Value	The content set to the "Value" on the [Access Data] tab is displayed.	
(1) (Comment data)	Set the comment data to be used for the comment display function.	Page 114 Comment data
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Comment data

■"Range (Lower)" and "Range (Upper)"

Set the lower and upper limit values of the device.

The setting range changes depending on the data type.

The following table shows the setting range of each data type.

Data type	Setting range
Bit	1 (ON), 0 (OFF)
16 bit integer	-32768 to 32767
32 bit integer	-2147483648 to 2147483647

■"Comment String"

Enter the comment character string to be displayed in the cell.


Number of characters: up to 40

■"Character Color"

Set the color of the comment character string displayed in the cell.

Depending on the specified colors, all colors may turn to gray.

For details, refer to the following:

 Page 12 Considerations for setting MX Sheet

Point

If multiple comment data is set and their setting ranges are overlapped, the comment character string with the lowest data number is displayed.

Be sure to prevent double setting of the setting ranges.

Setting examples


The following shows the setting examples in the cases where the data type is set to "Bit" and "16 bit integer".

■When data type is set to "Bit"

- [Comment Data] tab setting example

Device	M0	Data Type	Bit	Value	DEC
		Range(Lower)	Range(Upper)	Comment String	Character Color
1	0	0		Normal operation	
2	1	1		Error occurrence	
3					

- Operation of M0

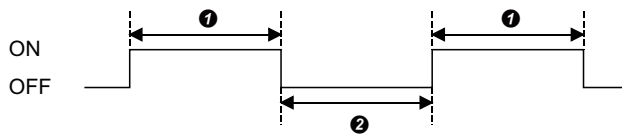


- ① While M0 is ON, "Error occurrence" is displayed in the cell.
- ② While M0 is OFF, "Normal operation" is displayed in the cell.

■When data type is set to "16 bit integer"

- [Comment Data] tab setting example

Device	D0	Data Type	16bit integer	Value	DEC
		Range(Lower)	Range(Upper)	Comment String	Character Color
1	10000	32767		Temperature upper limit over	
2					
3					

- Operation of D0




- ① If the D0 value is 10000 or more, "Temperature upper limit over" is displayed in the cell.
- ② If the D0 value is less than 10000, no comment character string is displayed.

Setting of the [Operation Interval] tab

This section explains the setting of the [Operation Interval] tab for use of the comment display function. On the [Operation Interval] tab, set the day and time of the activation of the function for the cell area.

Window

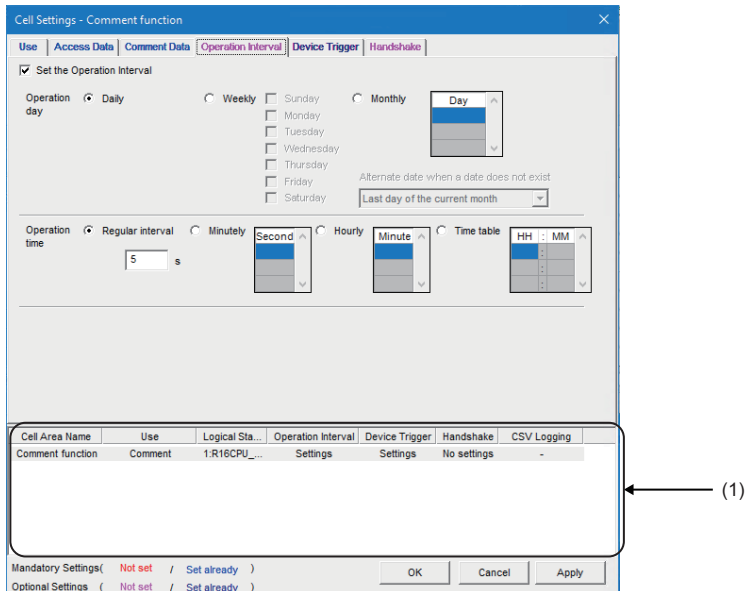

Displayed items

Item	Description	Reference
Set the Operation Interval	Set the operation of the cell area valid or invalid.	Page 62 "Set the Operation Interval"
Operation day	Set the operation day of the comment display function activation.	Page 62 "Operation day"
Operation time	Set the operation time of the comment display function activation.	Page 116 "Operation time"
(1) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

"Operation time"

The setting except for "Regular interval" is the same as that of the logging function.

☞ Page 63 "Operation time"

■When "Regular interval" is selected

Device data is collected at the set second intervals.

When setting lesser "seconds" than the actual communication time, the fixed interval communication cannot be established.

Hence, set for longer than the actual communication time.

For Communication time, refer to the following performance value.


☞ Page 161 Processing Speed of MX Sheet

Setting range: 0.001 to 0.999 (in units of 0.001 seconds), 1 to 3600 (in units of 1 second)

Setting of the [Device Trigger] tab

This section explains the setting of the [Device Trigger] tab for use of the comment display function. On the [Device Trigger] tab, set the device conditions for the device trigger.

Window

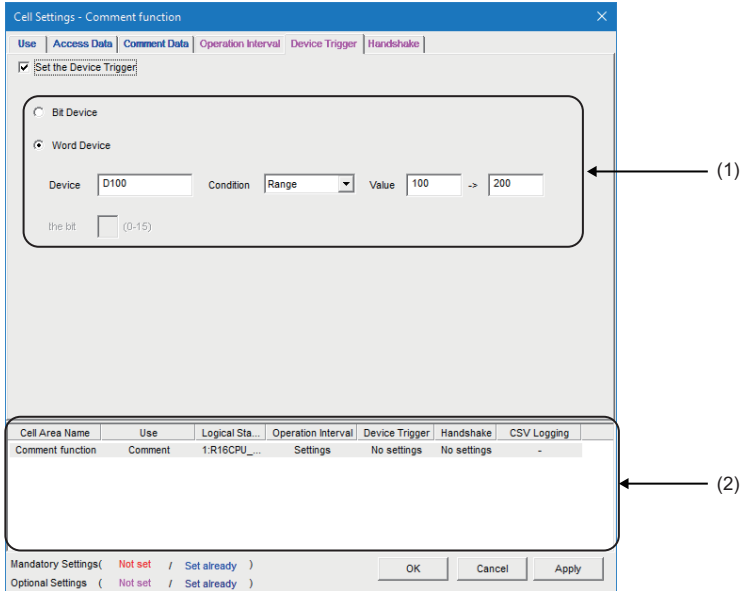


Displayed items

Item	Description	Reference
Set the Device Trigger	Set when the device trigger is used.	Page 67 "Set the Device Trigger"
(1) (Device conditions)	Set the device or label conditions.	Page 67 Device conditions
(2) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas

Setting of the [Handshake] tab

This section explains the setting of the [Handshake] tab for use of the comment display function. On the [Handshake] tab, set the handshake requesting source and handshake processing.

Window

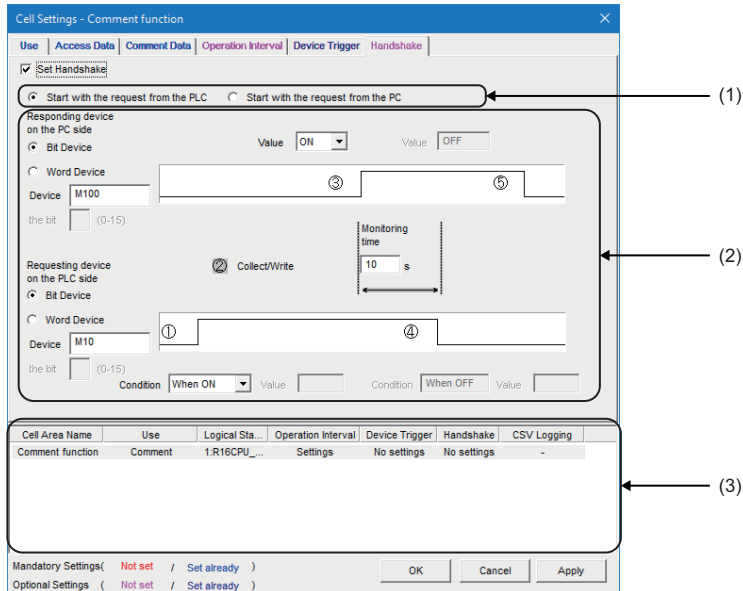

Displayed items

Item	Description	Reference
Set Handshake	Set when using a handshake.	Page 74 "Set Handshake"
(1) (Requesting source setting)	Set the requesting source of the handshake.	Page 74 Requesting source setting
(2) (Handshake processing)	Set the handshake processing.	Page 74 Handshake processing
(3) (Preset cell areas)	The settings of the cell areas preset to the Excel book are displayed.	Page 54 Preset cell areas


4 AUTOMATIC SAVE SETTING


This chapter explains the setting content for saving the Excel book or Excel spreadsheet (CSV format) during MX Sheet operation (hereafter abbreviated to the Automatic save setting data).

4.1 Operation of "Automatic Save List" Screen


Manage the automatic save conditions in the form of a list In the "Automatic Save List" screen.

Window



[MX Sheet] tab ⇨ [Automatic Save Setting] ()

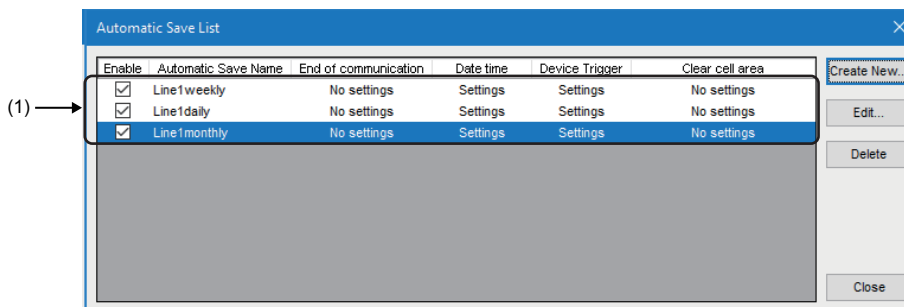

Displayed items

Item	Description	Reference	
(1) Automatic save name list	<ul style="list-style-type: none"> — Enable Automatic Save Name End of communication Date time Device Trigger Clear cell area 	<ul style="list-style-type: none"> Display a list of automatic save names created in the "Automatic Save" screen ( Page 120 Setting of "Automatic Save" Screen). Select the checkbox of a target for automatic saving. Selected when new data is created. Display the automatic save names created in the "Automatic Save" screen. Display whether the "Save at the end of communication" check box in the "Automatic Save" screen is selected or not in the form of Settings or No settings. Display whether the "Set the date and time" check box in the "Automatic Save" screen is selected or not in the form of Settings or No settings. Display whether the "Set the Device Trigger" check box in the "Automatic Save" screen is selected or not in the form of Settings or No settings. Display whether the "Clear cell area after automatic save" check box in the "Automatic Save" screen is selected or not in the form of Settings or No settings. 	—
[Create New] button	Display the "Automatic Save" screen and create new automatic save setting data.	Page 120 Setting of "Automatic Save" Screen	
[Edit] button	Display the "Automatic Save" screen and change the content of the existing automatic save setting data.	—	
[Delete] button	Delete the selected automatic save name from the automatic save name list.	—	

Point

- When the automatic save name list is double-clicked or the  key is pressed with the clicked line highlighted, that operation has the same function as the [Edit] button.
- When the  key is pressed with the clicked line highlighted, that operation has the same function as the [Delete] button.

4.2 Setting of "Automatic Save" Screen

Set the save timing and file name on the "Automatic Save" screen.

Point

Save timing

The following three save timings are available for the automatic save setting. (All of them can be set at a time.)

- Automatic save is performed at the end of communication.
- Automatic save is performed at a specified time.
- Automatic save is performed using the device trigger.

Window

Click the [Create New] button or the [Edit] button on the "Automatic Save List" screen.

Displayed items

Item	Description	Reference
Automatic Save Name	Attach specific names to the automatic save setting data. Up to 50 automatic save names can be registered.	—
Save at the end of communication	Set when performing automatic save at the end of communication.	
Set the date and time	Set when performing automatic save at the specified date and time.	
Operation day	Set the operation day when automatic save is performed at the specified date and time.	Page 121 "Operation day"
Operation time	Set the operation time when automatic save is performed at the specified date and time.	Page 121 "Operation time"
Set the Device Trigger	Set this when performing automatic save using the device trigger.	Page 122 "Set the Device Trigger"
(1) (Device conditions)	Set the device conditions for the device trigger.	Page 122 Device conditions
Clear cell area after automatic save	Set when clearing the cell area data after automatic save.	Page 123 "Clear cell area after automatic save"
Specify the cell area name	From the list, select the cell area name that is the target of "Clear cell area after automatic save".	Page 123 "Specify the cell area name"
(2) (Save file setting)	Set the file name to automatically save data.*1	Page 123 Save file setting
Add device data to File Name	Set when adding device data to the file name automatically saved.*2	Page 124 "Add device data to File Name"

Item	Description	Reference
(3) (Device setting)	Set device data to be added to the file name automatically saved.	Page 124 Device setting
[OK] button	Register the newly created or edited "Automatic Save Name" to the "Automatic Save List" screen.	Page 125 Registration of an "automatic save name"

*1 A UNC path name (\\server name\path name) cannot be specified as a file name. After assigning the network drive, specify the path name.

*2 Can be selected only when "Fix the File name" is set for (2) (Save file setting).

Point

When "Clear cell area at the start of communication" is checked on the [Use] tab of the "Cell Settings" screen, MX Sheet clears the target cell area data at the start of communication and starts data collection. In order to save the data at the end of communication, select the checkbox of "Save at the end of communication".

"Operation day"

Set the operation day of the automatic save function.

■When "Daily" is selected

Save is performed every day.

■When "Weekly" is selected

Save is performed on the specified day of the week only.

Multiple days of the week can be set.

■When "Monthly" is selected

Save is performed on the specified days only.

If the specified day does not exist in some months, an alternate day can be specified.

Number of days that can be set: 31

- When "15th" is set

Operation is performed on the 15th every month, e.g. January 15, February 15, March 15.

- When "31st" is set

Excepting February, April, June, September and November, operation is performed on the 31st every month.

For February, April, June, September and November, set the alternate day and processing in "Alternate day when a date does not exist".

The following table shows the setting items of "Alternate day when a date does not exist".

Item	Description
Last day of the current month	Operation is performed on the last day of February, April, June, September or November.
First day of the next month	Operation is performed on the first day of the next month.
No operation	Operation is not performed in February, April, June, September and November.

"Operation time"

Set the operation time of automatic save.

■When "Regular interval" is selected

The Excel book is saved at the set minute intervals.

Setting range: 1 to 1440

- When "Regular interval" is set to "5"

The Excel book is saved at intervals of 5 minutes, e.g. 8:05, 8:10, 8:15.

■When "Hourly" is selected

Automatic save is performed at the specified minute every hour.

Number of times that can be set: 60

■When "Time table" is selected

Automatic save is performed at the specified time.

Number of times that can be set: 50

"Set the Device Trigger"

Set this when performing automatic save using the device trigger.

Whether the device trigger conditions are satisfied or not is checked at intervals of 1 second.

Device conditions

■"Logical Station Number"

Select the logical station number used for the device trigger.

If the logical station number is already set, the number is displayed in the list box and can be selected.


If the logical station number is not set, click the [Communication Settings] button and set a new logical station number.

Point

The "Remote password" screen is displayed when the setting of the logical station number selected in "Logical Station Number" includes information on the connection to the module with the password function. Enter the password when the password is set to the connection target CPU module. It need not be entered when the password is not set.

■[Communication Settings] button

Click this to start Communication Settings Utility for setting a new logical station number and changing settings.

Select "Run as administrator" when the "User Account Control" screen ( Page 176 Warning Messages on Windows) asking if execute programs with administrator authority or not appears.

After starting Communication Settings Utility, click the [Wizard] button and set a new logical station number and change the settings with Communication Setting Wizard.

For the detailed explanation of Communication Settings Utility and Communication Setting Wizard, refer to the following:

 MX Component Version 5 Reference Manual

■Device type

Set the type of the device used for the device trigger.

Item	Description
Bit device	Set when using a bit device for the device trigger.
Word device	Set when using a word device for the device trigger.

■"Device"



Enter the device or label used for the device trigger.

Item	Description
When using a device*1	Enter a device name and device number in this order.
When using a label*1	Enter a label name. The applicable data types is Bit. When entering a label, enter other than structured data type label and array type label.

*1 Z device and TN/CN/STN devices cannot be used.

■"Condition"

Set the device trigger condition.

Item	Available Device	Description
When ON 	Bit device	Set when automatic save is to be performed when the bit device turns ON.
	Word device	Set when automatic save is to be performed when the corresponding bit of the word device turns ON (value: 1).
When OFF 	Bit device	Set when automatic save is to be performed when the bit device turns OFF.
	Word device	Set when automatic save is to be performed when the corresponding bit of the word device turns OFF (value: 0).

■"the bit"

Set the corresponding bit of the word device.

Setting range: 0 to 15

"Clear cell area after automatic save"

Set whether the data of the cell area selected in the "Specify the cell area name" is cleared or not after automatic save is performed.

To clear the cell area data after automatic save, select the check box.

"Specify the cell area name"

From the list box, select the "Cell Area Name" of the cell area whose data is cleared after automatic save. (Multiple names can be selected.)

The list box displays all cell area names set in the "Cell Settings" screen.

Save file setting

■"File name to save"

Set the storage location and file name of the Excel book to be saved automatically.

The Excel file (.xls, .xlsx, .xlsm, .xlsb)*¹, HTML file (.htm), or CSV file (.csv) can be set as the file type.*²

*1 An Excel file can be set only with the same extension as the file in which MX Sheet is set.

*2 For the continuous operation when saving data automatically in a file, refer to the following:

☞ Page 14 Continuous operation of Excel

■"Specify the sheet name"


Select the sheet name to be saved from the combo box.

It can be specified only when the "File name to save" is a CSV file.

■"Add date and time to File name"

The file set in "File name to save" saves data with the date and time added to its file name.

The following shows a file name format when data is saved.

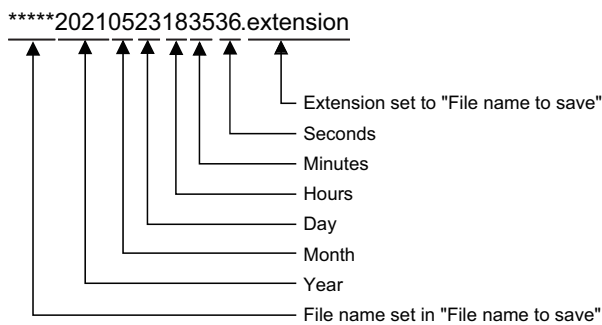


■"Add sequential number to File name"

The file set in "File name to save" saves data with a number added to its file name.

A serial number can be set within the range from 000 to 999.

When the number reaches the last, the data of the next file are overwritten to the file of the first number.

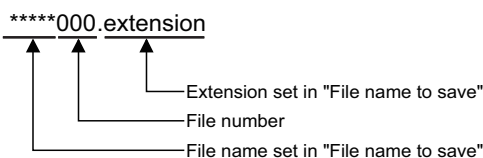


■"Fix the File name"

Data is overwritten to the file set in "File name to save."

"Add device data to File Name"

Set when adding device data to the file name automatically saved.

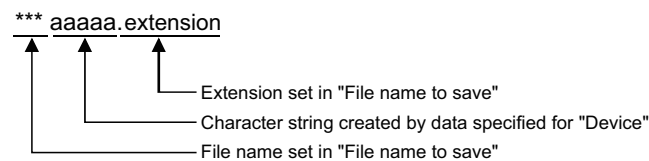

Device setting

■"Logical Station Number"

Select the logical station number of the device used for the file name.

If the logical station number is already set, the number is displayed in the list box and can be selected.


If the logical station number is not set, click the [Communication Settings] button and set a new logical station number.

Point

The "Remote password" screen is displayed when the setting of the logical station number selected in "Logical Station Number" includes information on the connection to the module with the password function. Enter the password when the password is set to the connection target CPU module. It need not be entered when the password is not set.

■[Communication Settings] button

Click this to start Communication Settings Utility for setting a new logical station number and changing settings.

Select "Run as administrator" when the "User Account Control" screen ( Page 176 Warning Messages on Windows) asking if execute programs with administrator authority or not appears.

After starting Communication Settings Utility, click the [Wizard] button and set a new logical station number and change the settings with Communication Setting Wizard.

For the detailed explanation of Communication Settings Utility and Communication Setting Wizard, refer to the following:

 MX Component Version 5 Reference Manual

■"Device"

Specify the device name or label name to be used for the file name.

Bit devices cannot be specified.

■"Data Type"

Select the type of data to be read from the device in the following:

- 16 bit integer
- 32 bit integer
- Character string

When "Character string" is selected for "Data type", the read data is processed as Shift JIS code.

■"Value"

Select the display format of the value to be displayed from DEC and HEX.

When "Character string" is selected for "Data type", it cannot be specified.

■"No. of characters"

Specify the number of characters to be read to one unit of data from the specified device.

It can be specified only when selecting "Character string" for "Data type".

Setting range: 1 to 40

Registration of an "automatic save name"

Register the newly created or edited automatic save setting data.

When the registration is completed, the automatic save name and settings are displayed as shown below in the "Automatic Save List" screen.

Operation		Display in "Automatic save list"
Create New		The automatic save name and settings are additionally displayed at the bottom of the list, and "Enable" is selected.
Edit	When automatic save name is changed	The automatic save name and settings are additionally displayed at the bottom of the list, and "Enable" is selected.
	When automatic save name is the same	The automatic save name and settings are displayed in the same position of the list. When the settings are changed, the new settings are displayed.

Point

When registering the existing automatic save setting data under a different automatic save name, change the automatic save name in the "Automatic Save" screen.


5 AUTOMATIC PRINT SETTING


The following explains the setting content for printing the Excel book or Excel spreadsheet (CSV format) during MX Sheet operation (hereafter abbreviated to the Automatic print setting data).

5.1 Operation of "Automatic Print List" screen


Manage the automatic print conditions in the form of a list in the "Automatic Print List" screen.

Window

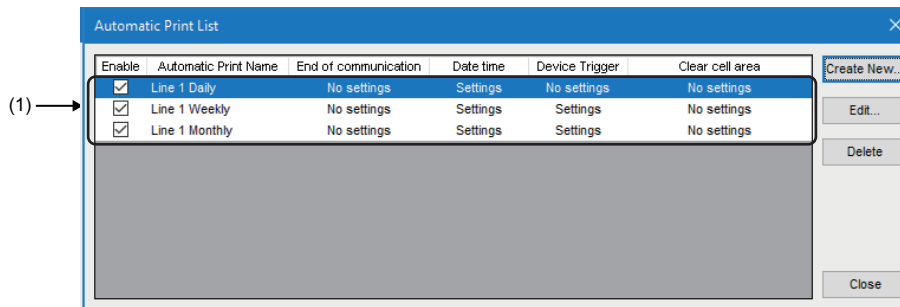

[MX Sheet] tab ⇨ [Automatic Print Setting] ()



Displayed items

Item	Description	Reference
(1) Automatic print name list	<p>—</p> <p>Display a list of automatic print names created on the "Automatic Print" screen ( Page 127 Setting of "Automatic Print" Screen).</p> <p>Enable</p> <p>Select the checkbox of an item for automatic printing. Selected when new data is created.</p> <p>Automatic Print Name</p> <p>Display the automatic print name created on the "Automatic Print" screen.</p> <p>End of communication</p> <p>Display whether the "Print at the end of communication" check box in the "Automatic Print" screen is checked or not in the form of Settings or No settings.</p> <p>Date time</p> <p>Display whether the "Set the date and time" check box in the "Automatic Print" screen is checked or not in the form of Settings or No settings.</p> <p>Device Trigger</p> <p>Display whether the "Set the Device Trigger" check box in the "Automatic Print" screen is checked or not in the form of Settings or No settings.</p> <p>Clear cell area</p> <p>Display whether the "Clear cell area after automatic print" check box in the "Automatic Print" screen is checked or not in the form of Settings or No settings.</p>	—
[Create New] button	Display the "Automatic Print" screen and create new automatic print setting data.	Page 127 Setting of "Automatic Print" Screen
[Edit] button	Display the "Automatic Print" screen and change the content of the existing automatic print setting data.	—
[Delete] button	Delete the selected automatic print name from the automatic print name list.	—

Point

- When the automatic print name list is double-clicked or the  key is pressed with the clicked line highlighted, that operation has the same function as the [Edit] button.
- When the  key is pressed with the clicked line highlighted, that operation has the same function as the [Delete] button.

5.2 Setting of "Automatic Print" Screen

Set the print timing and print area in the "Automatic Print" screen.

Point

Print timing

The following three timings are available for the automatic print setting. (All of them can be set at a time.) For the details, refer to the following:

☞ Page 119 AUTOMATIC SAVE SETTING

- Automatic print is performed at the end of communication.
- Automatic print is performed at a specified time.
- Automatic print is performed using the device trigger.

Window

Click the [Create New] button or the [Edit] button on the "Automatic Print List" screen.

5

Item	Description	Reference
Automatic Print Name	Manage the automatic print setting data with specific names. Up to 50 automatic print names can be registered.	—
Print at the end of communication	Set when performing automatic print at the end of communication.	Page 126 Operation of "Automatic Print List" screen
Set the date and time	Set when performing automatic print at the specified date and time.	
Operation day	Set the operation day when automatic print is performed at the specified date and time.	
Operation time	Set the operation time when automatic print is performed at the specified date and time.	
Set the Device Trigger	Set when performing automatic print using the device trigger.	
(1) (Device conditions)	Set the device conditions for the device trigger.	
Clear cell area after automatic print	Make setting when clearing the cell area data after automatic print.	Page 128 "Clear cell area after automatic print"
Specify the cell area name	From the list, select the cell area name that is the target of "Clear cell area after automatic print".	Page 128 "Specify the cell area name"
Print Area	Set the area where automatic print is performed.	Page 128 "Print Area"
[OK] button	Register the newly created or edited "Automatic Print Name" in the "Automatic Print List" screen.	Page 128 Registration of an "automatic print name"

"Clear cell area after automatic print"

Set whether the data of the cell area selected in the "Specify the cell area name" is cleared or not after automatic print is performed.

To clear the cell area data after automatic print, select the check box.

"Specify the cell area name"

From the list box, select the "Cell Area Name" of the cell area whose data is cleared after automatic print. (Multiple names can be selected.)

The list box displays all cell area names set in the "Cell Settings" screen.

"Print Area"

Set the area where automatic print is performed.

■"Entire workbook"

The entire Excel book (all sheets) where automatic print setting is set is printed automatically.

■"Specify the sheet"

Automatic print is executed for the specified sheet only.

Multiple sheets can be selected and printed simultaneously.

Registration of an "automatic print name"

Register the newly created or edited automatic print setting data.

When the registration is completed, the automatic print name and settings are displayed in the "Automatic Print List" screen as described below.

Operation		Display in "Automatic print list"
Create New		The automatic print name and settings are additionally displayed at the bottom of the list, and "Enable" is selected.
Edit	When automatic print name is changed	The automatic print name and settings are additionally displayed at the bottom of the list, and "Enable" is selected.
	When automatic print name is the same	The automatic print name and settings are displayed in the same position of the list. When the settings are changed, the new settings are displayed.

Point

- When registering the existing automatic print setting data under a different automatic print name, change the automatic print name in the "Automatic Print" screen.
- When multiple printers are set to a single personal computer, the Excel spreadsheet where automatic print is set is output from the printer specified to "Set as Default" in [Devices and Printers] of [Hardware and Sound] in the control panel of Windows.

6 AUTOMATIC COMMUNICATION STARTUP/ CANCELLATION

This chapter explains the procedure for registering settings for starting communication with a CPU module automatically at the start of the Excel book.

In addition, this chapter explains the procedure for cancelling the automatic communication startup setting.

6.1 "Automatic Communication Startup"

Operating procedure

1. Select the [Automatic Communication Startup] checkbox in the [MX Sheet] tab.
2. Click the [Yes] button in the displayed screen to register the automatic communication startup setting to the Excel book being edited.
3. Click the [OK] button in the displayed screen.

After editing the Excel book, restart the Excel book to enable the automatic communication startup setting.

6.2 Cancelling "Automatic Communication Startup"

Operating procedure

1. Unselect the [Automatic Communication Startup] checkbox in the [MX Sheet] tab.
2. Click the [Yes] button in the displayed screen to cancel the automatic communication startup setting of the Excel book being edited.

Point



- For setting the automatic communication startup setting, do not save the Excel book under the hidden status.

An error occurs when starting the Excel book and MX Sheet cannot be used. In such case, save the Excel book under the display status, and restart Excel.

For the method to display the Excel book, refer to the corrective action of "When MX Sheet setting is set, only the frame of Excel is displayed." in the following troubleshooting:

☞ Page 177 Troubleshooting

- When opening an Excel book where the automatic communication startup setting is set in Microsoft Excel 2007 or later, the following symptoms may occur:
 - Excel stops responding.
 - One of the following error messages is displayed.

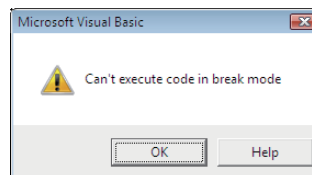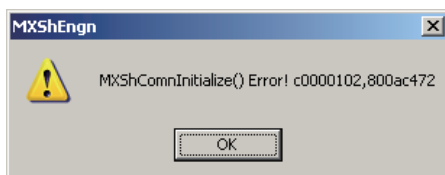

If the symptoms described above occur, refer to the following appendix and install the COM add-in "MX Sheet Ribbon Add-in."

☞ Page 179 Countermeasures for errors as a result of setting the automatic communication startup setting in an Excel book and opening it in Microsoft Excel 2007 or later

7 START COMMUNICATION AND END COMMUNICATION

This chapter explains the start and end of MX Sheet communication.

7.1 Start Communication

This section explains the procedure to start MX Sheet communication manually.

Operating procedure

1. [MX Sheet] tab ⇒ [Start] (🖨️)
2. Click the [Yes] button in the displayed screen.

Start communication between the Excel book being edited, and a CPU module and read/write device data.

Point


- The communication can be also started by clicking the created start communication button. (🖨️ Page 143 Start Communication Button)
- Do not operate other Excel book during communication.
- An Excel book is protected during communication. When not protecting an Excel book, change the option setting. (🖨️ Page 155 Protecting a workbook)
- If an Excel book is accidentally protected due to the forced termination of Excel during communication etc., unprotect the workbook in the [Review] tab of Excel. A password is not set for the workbook protection function during communication.

Display of Excel book and task bar during communication

The following shows how the Excel book, which is communicating with a CPU module using MX Sheet, and the task bar are displayed.

■ Display of Excel book

Window

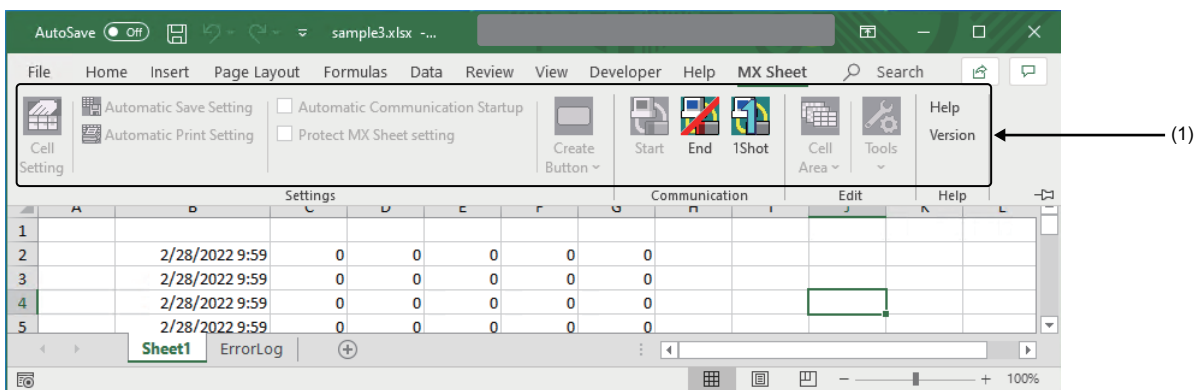

Item	Status during Communication
(1) Menu, icons	Only the following items are available: "End," "1Shot," "Help," and "Version."

■ Display of task bar

During communication with a CPU module using MX Sheet, the icon (🖨️) is displayed on the task bar of Windows.

Confirmation at communication error

If an error occurs at the start of communication or during communication, the error information is displayed on the "ErrorLog" sheet.

When a communication error has occurred, end MX Sheet communication and correct the error in accordance with the corrective action on the "ErrorLog" sheet.

For details of the "ErrorLog" sheet, refer to the following chapter.

☞ Page 153 "ErrorLog" sheet

Kind	Date	Cell Area Name	ErrorNo	Contents
Error	2022/02/17 Thu 12:40:05	logging	e1000009	The specified logical station number is not set. The corrective action is as follows: Create the logical station number after performing communication setting.
Information	2022/02/17 Thu 12:43:08		00000002	Communication was completed.

At occurrence of communication error, error information is displayed on the "ErrorLog" sheet.

7.2 End Communication

This section explains the procedure to end MX Sheet communication.

Operating procedure

[MX Sheet] tab ⇨ [End] (🗑️)

Point

- The communication can also be ended by clicking the created end communication button. (📖 Page 147 End Communication Button)


Confirmation at communication end

At the end of communication, MX Sheet displays the communication end message on the "ErrorLog" sheet.

Confirm the message on the "ErrorLog" sheet at the end of communication.

For details of the "ErrorLog" sheet, refer to the following chapter.

📖 Page 153 "ErrorLog" sheet

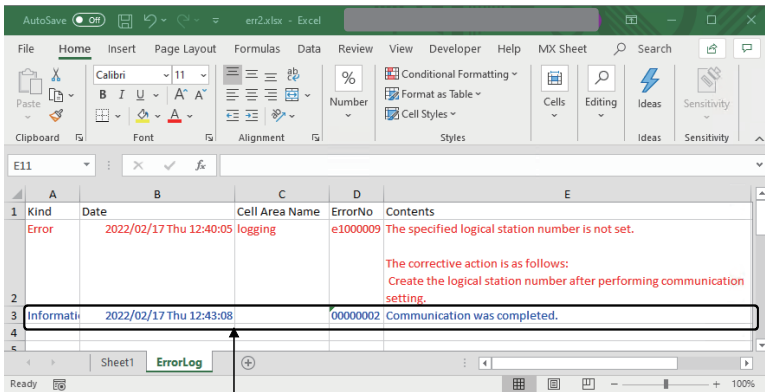

At end of communication, communication end message is displayed on "ErrorLog" sheet.

8 1 SHOT COMMUNICATION



This chapter explains 1 shot communication function that makes communication with the selected cell area only once at any timing.


The "1Shot Communication" screen is used to set a cell area and execute 1 shot communication for the cell area.

Point

- 1 shot communication function ignores the device trigger and handshake settings set to the cell area, and performs communication only once.
- 1 shot communication function cannot work with the alarm summary function.

Window

- [MX Sheet] tab ⇒ [1Shot] ()
- Click the 1 shot communication button. ( Page 148 1 Shot Communication Button)

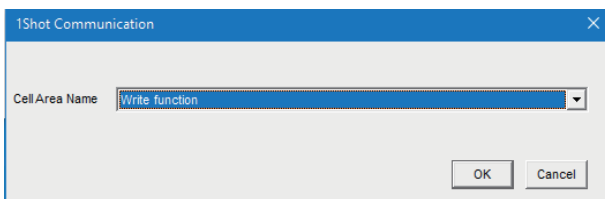

Displayed items

Item	Description
Cell Area Name	Select the cell area for 1 shot communication. Only the cell area name set in the currently selected Excel spreadsheet is displayed in "Cell Area Name".
[OK] button	The button can be clicked after the cell area name is selected in "Cell Area Name". Execute 1 shot communication.

Point

- When "1Shot Communication" screen is activated after selecting the cell area set on the Excel spreadsheet with the mouse, the cell area name of the selected cell area is displayed on "Cell Area Name".
- Setting the cell area name in "Cell Area Name" displays the cell area on the Excel spreadsheet.

MEMO


9 EDITING CELLS


This chapter explains how to edit the cell area set using MX Sheet.

9.1 Cutting Cell Area

This section explains the procedure to delete the settings of the selected cell area and paste them to another cell area.

Window

[MX Sheet] tab ⇒ [Cell Area] ⇒ [Cut Cell Area] ()

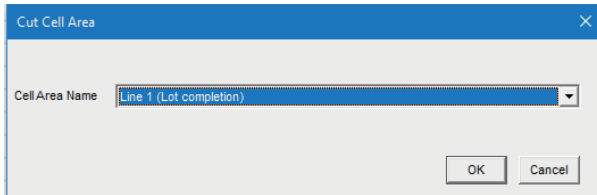


Displayed items

Item	Description
Cell Area Name	Select the cell area name to be cut.
[OK] button	Cut the cell area. The button can be clicked after the cell area name is selected in "Cell Area Name".

Point


For pasting the cell area, refer to the following:


 Page 138 Pasting Cell Area

9.2 Copying Cell Area

This section explains the procedure to copy the settings of the selected cell area to another cell area.

Window

[MX Sheet] tab ⇒ [Cell Area] ⇒ [Copy Cell Area] ()

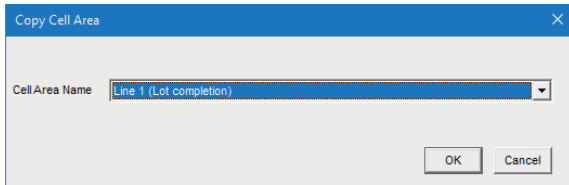


Displayed items

Item	Description
Cell Area Name	Select the cell area name to be copied.
[OK] button	Copy the cell area. The button can be clicked after the cell area name is selected in "Cell Area Name".

Point


For pasting the cell area, refer to the following:


 [Page 138 Pasting Cell Area](#)

9.3 Pasting Cell Area

This section explains the procedure to paste the cut or copied cell area to another cell area.

Window

[MX Sheet] tab ⇨ [Cell Area] ⇨ [Paste Cell Area] ()

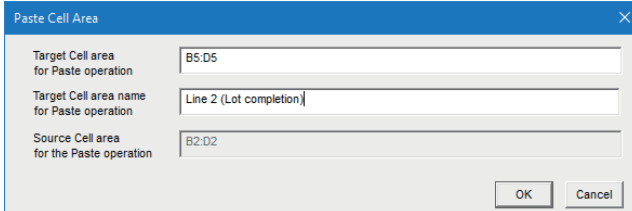

Displayed items

Item	Description
Target Cell area for Paste operation	Enter the cell area to be pasted.
Target Cell area name for Paste operation	Enter the cell area name to be pasted. ^{*1}
Source Cell area for the Paste operation	The cut or copied cell area is displayed.
[OK] button	Paste the cell area. The button can be clicked after setting "Target Cell area for Paste operation" and "Target Cell area name for Paste operation".

*1 When pasting the cell area after copying it, enter into "Target Cell area name for Paste Operation" the cell area name that differs from the copied cell area name.

Point


The cell area cannot be pasted unless the cell area is selected by cutting or copying it.

Considerations for pasting the cell

Consider the following when pasting a cell area.

■ Paste starting cell in cell area


The paste starting cell in the cell area is the cell selected on the Excel spreadsheet.

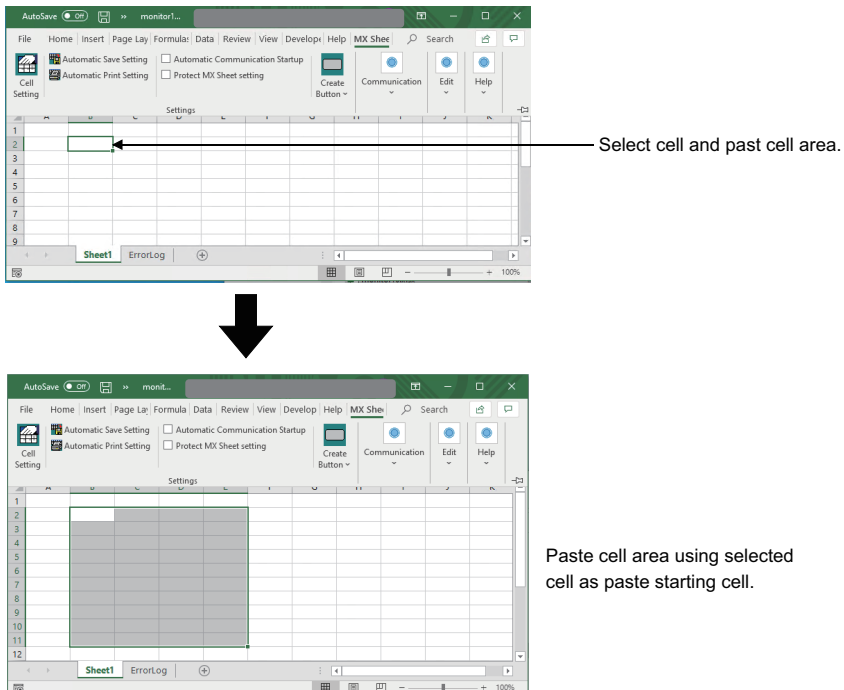

■ Overlap of cell areas

If the paste area overlaps the other cell area that is already set, the selected cell cannot be pasted.

Paste the cell after checking the other cell area.

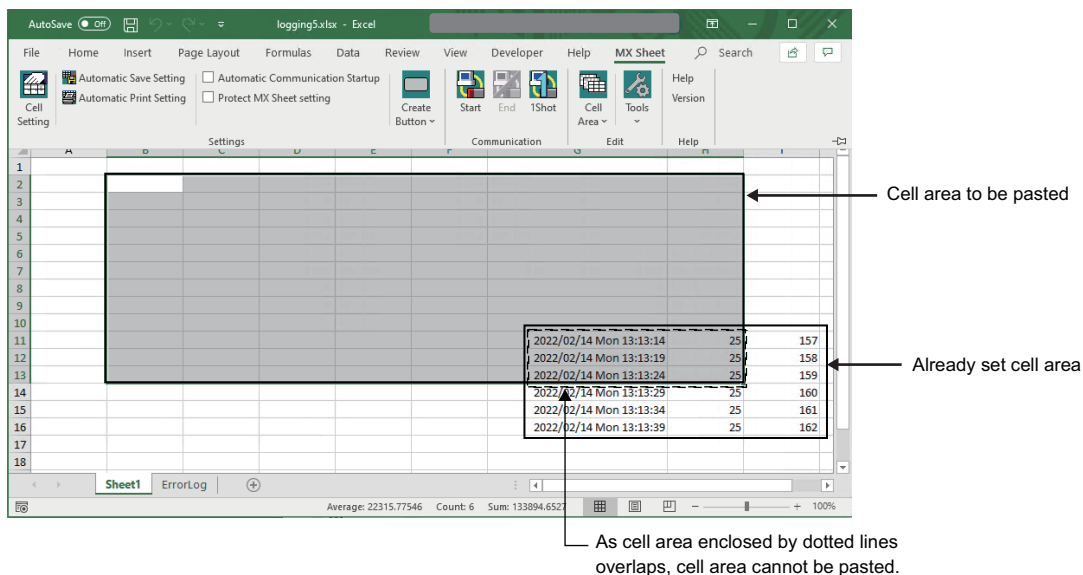


Point


The cell can be pasted when both of the following conditions are met: the area of "Already set cell area" and "Cell area to be pasted" are completely matched, and "Monitor" and "Write" are set to "Use" on each "Cell Settings" screen.

9.4 Deleting Cell Area

This section explains the procedure to delete the settings of the cell area.

Window

[MX Sheet] tab ⇨ [Cell Area] ⇨ [Delete Cell Area] ()

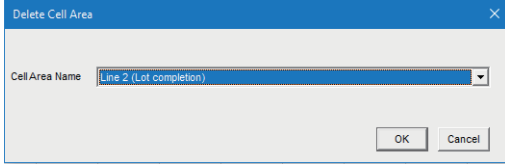

Displayed items

Item	Description
Cell Area Name	Select the cell area name to be deleted.
[OK] button	Delete the cell area. The button can be clicked after the cell area name is selected in "Cell Area Name".

10 CHANGING SHEET NAME

This chapter explains the changing the sheet name of the Excel spreadsheet where MX Sheet is set. In the "Change Sheet Name" screen, select an Excel spreadsheet and set a new name for the sheet.

10


Point

Always change the sheet name of the Excel spreadsheet, where MX Sheet is set, from the "Change Sheet Name" screen.

If the sheet name is changed from Excel directly or from a VBA program, MX Sheet does not operate normally.

Window

[MX Sheet] tab ⇒ [Tools] ⇒ [Change Sheet Name] (🔗)

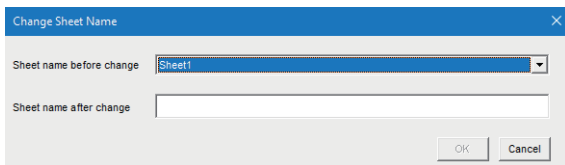

Displayed items

Item	Description
Sheet name before change	Select the Excel spreadsheet of which sheet name to be changed.
Sheet name after change	Enter a new sheet name.
[OK] button	Change the sheet name. The button can be clicked after the "Sheet name before change" and "Sheet name after change" are selected.

Changing the sheet name

If the sheet name of the Excel spreadsheet, where MX Sheet is set, is changed from Excel directly or from a VBA program, return the sheet name to the old one from Excel.

If the sheet name is changed from the VBA program, delete the program part that changes the sheet name.

MEMO

11 CREATING BUTTONS

The following explains the Start Communication, End Communication and 1 Shot Communication execution button creation procedures and the property setting.



By merely clicking the created button, Start Communication, End Communication or 1 Shot Communication operation can be performed and easily operated.

11.1 Start Communication Button

Create the button for execution of Start Communication and paste it to an Excel spreadsheet.

Button pasting method

Operating procedure

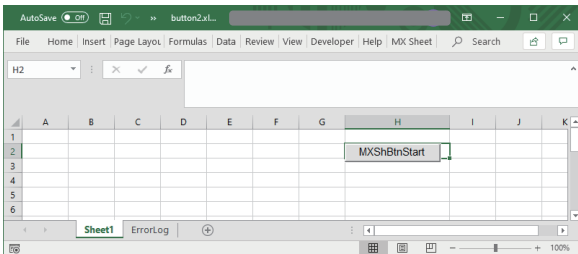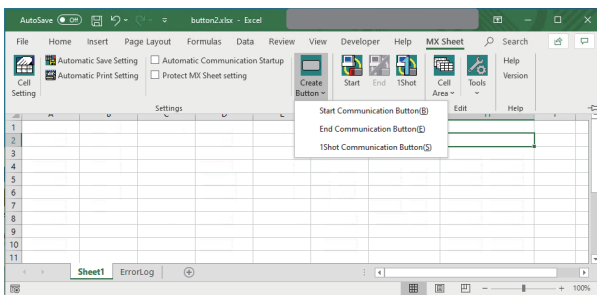

1. Specify a cell on an Excel spreadsheet where the button is to be placed, and select the [MX Sheet] tab ⇒ [Create Button] ⇒ [Start Communication Button].

The button is placed in the specified cell position.

2. The design mode is enabled in an Excel book immediately after the button is placed; therefore, disable it when clicking the button.

Point

The following settings about the placed button can be changed in the property setting.

- Changing the display characters on the button
- Changing the display/hidden status of the start message displayed when executing the button


For the details of the property setting, refer to the following:

👉 Page 144 Property page starting method

👉 Page 145 Property setting

Property page starting method



Operating procedure




1. Select [Design Mode] in the [Developer] tab to enter the design mode.

In order to display the [Developer] tab, select the [File] tab ⇒ [Options].

Select "Customize Ribbon" and check the "Developer" check box, and then click the [OK] button.

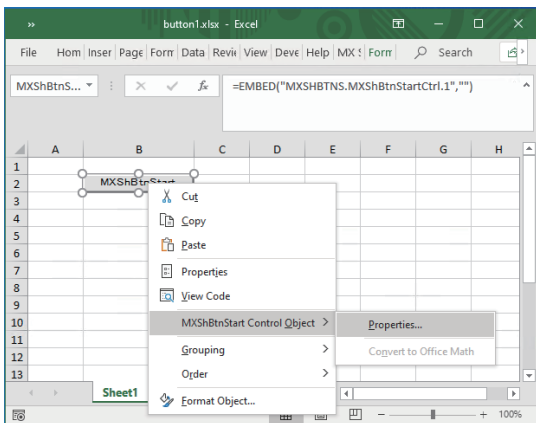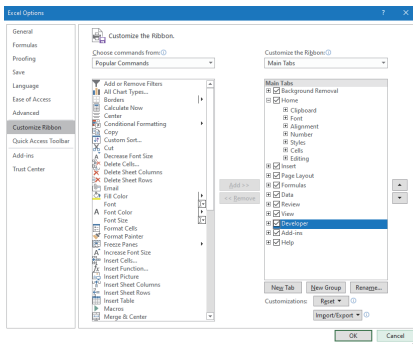

2. Select [MXShBtnStart Control Object] ⇒ [Properties] in the menu displayed by right-clicking the created button.

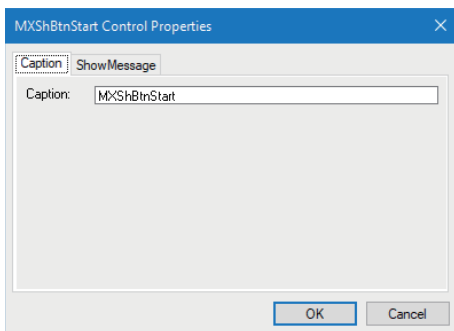

3. Start the property page.
For the property settings, refer to Page 145 Property setting.




When the property setting is completed, select [Design Mode] again to exit from the design mode.

Property setting

Set the each property of "Caption" and "ShowMessage."


■[Caption] tab

Edit the "Caption" (display characters on the button) of the button.

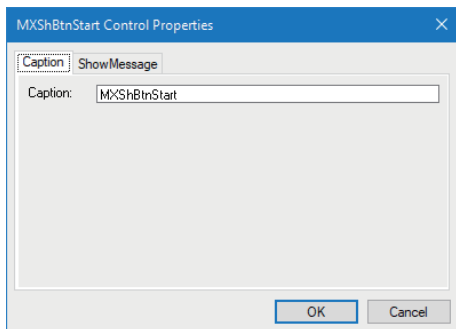

■[ShowMessage] tab

Set whether to display a confirmation message when clicking the start communication button.

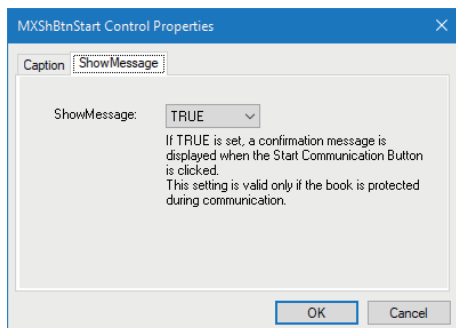

When selecting "TRUE," the following messages can be displayed according to option settings and the workbook protection status.

Item		Message
[MX Sheet] tab ⇒ [Tools] ⇒ [Options] ⇒ [Book Protect] tab ⇒ "Protect workbook while communicating"	Selected	
	Unselected	
When a workbook is already protected		

-
- Save the Excel book when the button is created or any property is changed.
 - Do not execute [Grouping] ⇔ [Ungroup] from the right-click menu of the button. Executing Ungroup disables the button from functioning.
 - If [Split], [Freeze Panes] or [New Window] in the [Window] menu is executed for the Excel spreadsheet where buttons is placed, correct operation may not be performed, e.g. the buttons remain displayed or the buttons cannot be clicked.
 - If the zoom of Excel is set to a large magnification, the button may be displayed above the row/column number. If it occurs, click the button. The button is then move to the correct position.
 - If a button is created in design mode and then the mode is ended and set repeatedly, the button may not be clicked.

In this case, minimize and restore the Excel book window. This enables the button to be clicked.

- When moving a button or changing button size after creating it, the button is not checked for its position.
 - If the button position exceeds the supported range (256 columns × 65536 rows) when Excel from 97 to 2003 version is saved in book format, any of the following occurs depending on the button size, button position, height of the row and/or cell width.
 - When saved Book is reopened, the button is reduced or moved so that it is fit within the supported range.
 - The button is deleted when saved Book is reopened.
 - The Compatibility Checker screen is displayed on the Excel at saving the Book.
-

11.2 End Communication Button

Create the button for execution of End Communication and paste it to an Excel spreadsheet.

Button pasting method

Same as the Start Communication Button.

☞ Page 143 Button pasting method

Operating procedure

[MX Sheet] tab ⇒ [Create Button] ⇒ [End Communication Button]

Property page starting method

Same as the Start Communication Button.

☞ Page 144 Property page starting method

Operating procedure

[MXShBtnEnd Control Object] ⇒ [Properties]

Property setting

Set the each property of "Caption."

☞ Page 145 Property setting

11.3 1 Shot Communication Button

Create the button for execution of 1 Shot Communication and paste it to an Excel spreadsheet.

Button pasting method

Same as the Start Communication Button.

☞ Page 143 Button pasting method

Operating procedure

[MX Sheet] tab ⇒ [Create Button] ⇒ [1Shot Communication Button]

Property page starting method

Same as the Start Communication Button.

☞ Page 144 Property page starting method

Operating procedure

[MXShBtn1Shot Control Object] ⇒ [Properties]

Property setting

Set the each property of "Caption" and "CellAreaName."

For Caption, refer to the following:


☞ Page 145 Property setting

■[CellAreaName] tab

The Cell Area Name list displays all Cell Area Names of Logging, Monitor, Write and Comment in the Excel book.

Select the check box for the Cell Area Name that is the target of 1 Shot Communication.


Up to 10 Cell Area Names can be selected.

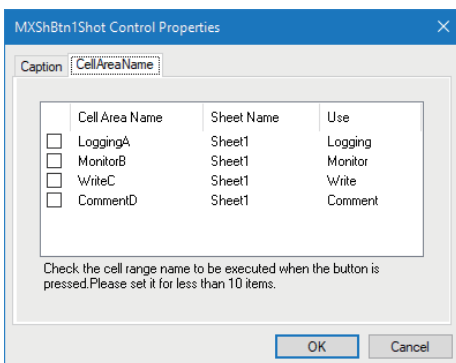

Point

If the following changes are made in the setting of Cell Area Name set for the 1 shot communication button, a warning message appears when clicking the 1 shot communication button. The warning message does not appear once the [CellAreaName] tab is opened.

- Cell Area Name is deleted in the cell setting.
- Cell Area Name is changed in the cell setting.
- Use is changed to the one that cannot be used for 1 Shot Communication in the cell setting.

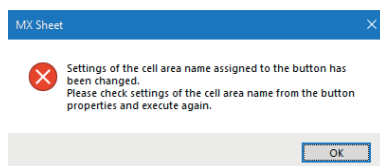

12 PROTECTING/UNPROTECTING MX Sheet SETTING

The following explains Protect MX Sheet setting and Unprotect MX Sheet setting by a password.


12.1 Protecting MX Sheet Setting

Protect the MX Sheet setting by a password so that the setting content cannot be changed.

The setting content cannot be edited until the MX Sheet setting is unprotected.

Window

Select the [Protect MX Sheet setting] checkbox in the [MX Sheet] tab.

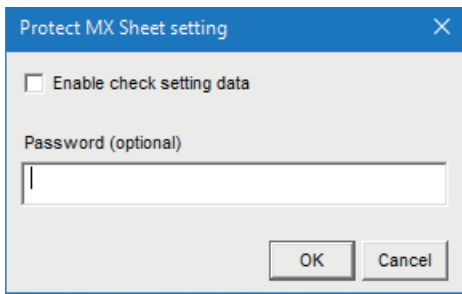

Displayed items

Item	Description	Reference
Enable check setting data	The menu that can be selected when Protect MX Sheet setting is set changes depending on if a check mark exists.	Page 150 "Enable check setting data"
Password (optional)	Enter the password for protecting the setting contents. The password may also be registered as a blank.	—
[OK] button	The "Confirm Password" screen is displayed. When the password is blank, however, the "Confirm Password" screen is not displayed and the MX Sheet setting is protected.	—

"Enable check setting data"

Depending on whether "the item is cleared" (setting content cannot be confirmed) or "Selected" (setting content can be confirmed), the menu that can be selected when Protect MX Sheet setting is set changes as shown in the following table.

○: Can be selected, ×: Cannot be selected

MX Sheet menu	Cleared	Selected
Cell Setting	×	○*1
Automatic Save Setting	×	○*1
Automatic Print Setting	×	○*1
Automatic Communication Startup	×	×
Unselecting "Protect MX Sheet setting" (checkbox)	○	○
Create Button (Start Communication Button, End Communication Button, and 1Shot Communication Button)	×	×
Start	○	○
End	○	○
1Shot	○	○
[Cell Area] ⇒ Cut Cell Area	×	×
[Cell Area] ⇒ Copy Cell Area	×	×
[Cell Area] ⇒ Paste Cell Area	×	×
[Cell Area] ⇒ Delete Cell Area	×	×
[Tools] ⇒ Change Sheet Name	×	×
[Tools] ⇒ Setting Data Export	×	×
[Tools] ⇒ Options	×	×
Help	○	○
Version Info.	○	○

*1 [Read only] is displayed after the title of the following screen related to the cell settings, automatic save setting and automatic print setting.

The setting content can be confirmed but cannot be changed.

- Cell Setting
- Automatic Save List
- Automatic Save
- Automatic Print List
- Automatic Print



If the MX Sheet setting is protected, the properties of the start communication button, end communication button, and the 1 shot communication button can be edited.

12.2 Unprotecting MX Sheet Setting


The MX Sheet setting is unprotected, and the setting content can be changed.

Point

When the password is not set in the "Protect MX Sheet setting" screen, the MX Sheet setting is unprotected without displaying the "Unprotect MX Sheet setting" screen.

Window

Unselect the [Protect MX Sheet setting] checkbox in the [MX Sheet] tab.

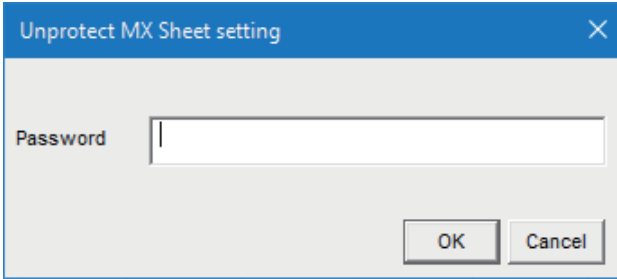


13 OPTIONS

Set option settings for the "ErrorLog" sheet output format and the workbook protection during communication.

13.1 Setting Error Logs


Set the "ErrorLog" sheet output format on the [Error log] tab on the "Options" screen.

For details of the "ErrorLog" sheet, refer to the following:


 Page 153 "ErrorLog" sheet

Window

[MX Sheet] tab ⇒ [Tools] ⇒ [Options] ⇒ [Error Log] tab

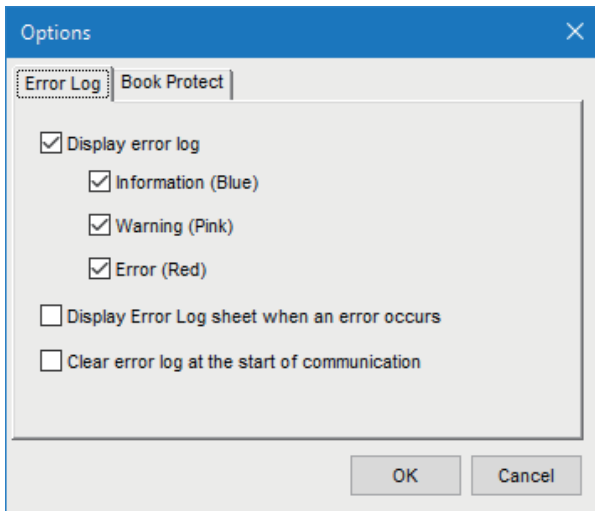

Displayed items

Item	Description
Display error log	—
	Set whether the information, warning, and error that occurred during the execution of communication is displayed on the "ErrorLog" sheet or not. <ul style="list-style-type: none"> • Selected: Displayed • No selected: Not displayed
	Information (Blue) *1
	Set whether the information message (blue) during the execution of communication is displayed on the "ErrorLog" sheet or not. <ul style="list-style-type: none"> • Selected: Displayed • No selected: Not displayed
	Warning (Pink) *1
	Set whether the warning message (pink) during the execution of communication is displayed on the "ErrorLog" sheet or not. <ul style="list-style-type: none"> • Selected: Displayed • No selected: Not displayed
	Error (Red) *1
	Set whether the error message (red) during the execution of communication is displayed on the "ErrorLog" sheet or not. <ul style="list-style-type: none"> • Selected: Displayed • No selected: Not displayed
Display Error Log sheet when an error occurs	Set whether the display is switched to the "ErrorLog" sheet or not if a warning or error occurs during the execution of communication. ( Page 153 "ErrorLog" sheet) <ul style="list-style-type: none"> • Selected: Display is switched to the "ErrorLog" sheet. • No selected: Display is not switched to the "ErrorLog" sheet.
Clear error log at the start of communication	Set whether the Error log is cleared or not at the start of communication. <ul style="list-style-type: none"> • Selected: Cleared • No selected: Not cleared

*1 Setting can be set only when the "Display error log" check box is selected.

"ErrorLog" sheet


The following explains the "ErrorLog" sheet that displays the communication status of MX Sheet.

The communication status, error information and corrective action of MX Sheet are displayed on the "ErrorLog" sheet.

Troubleshooting can be performed by confirming the corrective action displayed on the "ErrorLog" sheet.

Window

Select "ErrorLog" sheet in an Excel book.

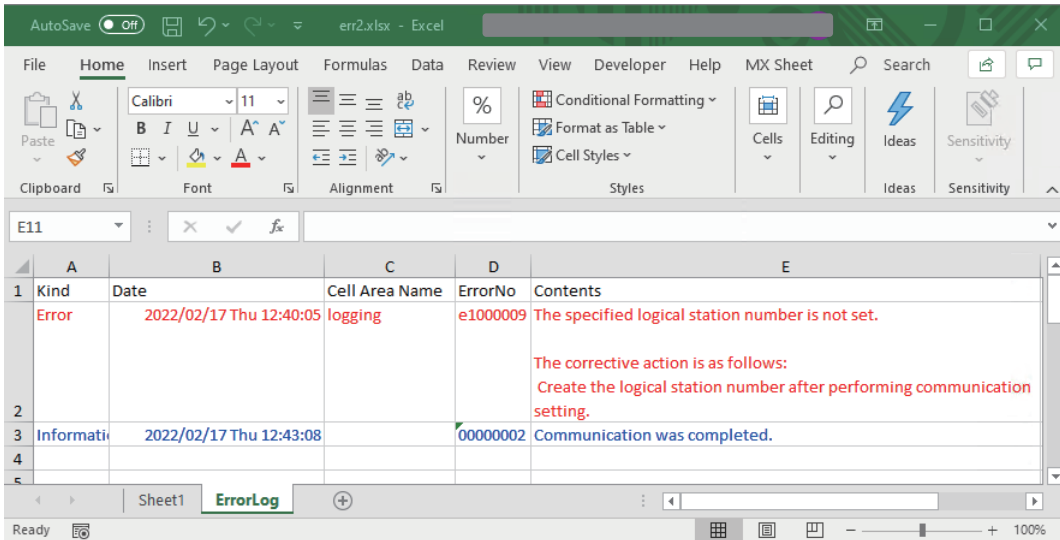

Displayed items

Item	Description	Reference
Kind	The type of the communication status is displayed.	Page 153 "Kind"
Date	The date and time when the communication status is changed are displayed. The displayed time is the date and time of the personal computer where MX Sheet is operating.	Page 154 "Date"
Cell Area Name	The cell area name where the communication status is changed is displayed.	Page 154 "Cell Area Name"
ErrorNo	The error number of the error that has occurred is displayed.	Page 154 "ErrorNo"
Contents	The details of the communication status is displayed. The error definition, error code and corrective action are displayed when an error occurs.	Page 154 "Contents"

"ErrorLog" sheet

The following table indicates the "ErrorLog" sheet specifications.

Item	Description
Maximum number of display lines	2000 lines (fixed)
New data location	The last line has the latest data.
Operation when cell is full	Overwritten in due order, starting with the first line.

"Kind"

The following table shows the communication status displayed in "Kind".

Communication Status	Description
Information	Displayed when the communication with a CPU starts and ends, and during 1 shot communication.
Error	Displayed when a fatal error occurred and the function of the cell area stopped.
Warning	Displayed when communication error or collection delay occurs.

"Date"

"Date" displays the date and time of the personal computer at "ErrorLog" sheet registration.

2021/05/23 Wed 18:31:06

(1) (2) (3)

(1) Indicates the date as "year/month/day".

(2) Indicates the day of the week as "Sun (Sunday), Mon (Monday), Tus (Tuesday), Wed (Wednesday), Thu (Thursday), Fri (Friday), Sat (Saturday)".

(3) Indicates the time as "hours: minutes: seconds".

"Cell Area Name"

The cell area name registered to the "ErrorLog" sheet is displayed.

It is not displayed when the communication starts and ends.

"ErrorNo"

The error number is displayed.

Specify the error number when inquiring about errors.

"Contents"

The data displayed in "Contents" are shown below.

Kind	Date	Cell Area Name	ErrorNo	Contents
Error	2022/02/17 Thu 12:40:05	logging	e1000009	The specified logical station number is not set.
				The corrective action is as follows: Create the logical station number after performing communication setting.
Information	2022/02/17 Thu 12:43:08		00000002	Communication was completed.

(1) Error definition is displayed.

(2) Corrective action for error is displayed.

Point

- If the same error occurs twice or more successively in the same cell area, only the error information of the first error is registered to the "ErrorLog" sheet. (The error information of the second error or later is not displayed.)
- Set the setting related to the "ErrorLog" sheet output format in the "Options" screen (Page 152 Setting Error Logs).

Checking method for the error codes output on an "ErrorLog" sheet

A message corresponding to the number in the ErrorNo column of the "ErrorLog" sheet is displayed in the Contents column. The following output example explains the codes included in the Contents column of the "ErrorLog" sheet.

Ex.

A communication error has occurred in communication of access data.

```
<00200104[Hex], 0180840b[Hex]>  
.....  
      (1)          (2)
```

(1) An internal number indicating the operation of MX Sheet

(2) A code of an error which occurs during communication

For details of error codes, refer to the following:

 MX Component Version 5 Reference Manual


13.2 Protecting a workbook

13

Set whether to protect a workbook during communication in the [Book Protect] tab in the "Options" screen.

Window

[MX Sheet] tab ⇒ [Tools] ⇒ [Options] ⇒ [Book Protect] tab

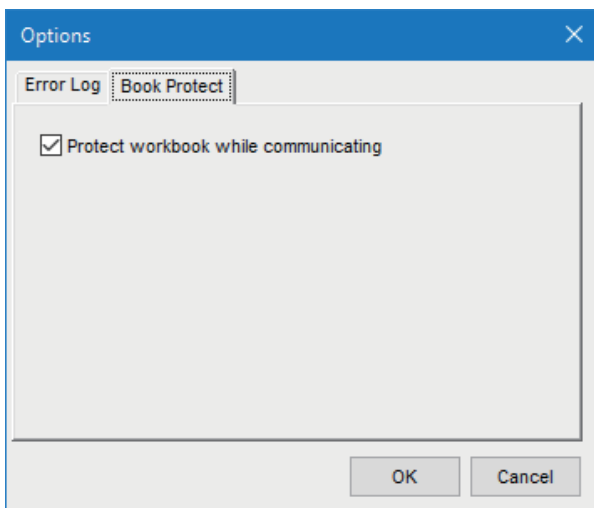

Displayed items

Item	Description
Protect workbook while communicating	Select the checkbox to protect an Excel book during communication. When an Excel book is already protected before the start of communication, the setting for this item is not applied.

Point

It is recommended to select the checkbox of "Protect workbook while communicating" in order to prevent incorrect operation during communication.

14 EXPORTING SETTING DATA

This chapter explains the procedure to output the settings of MX Sheet to a CSV file.

Operating procedure

[MX Sheet] tab ⇒ [Tools] ⇒ [Setting Data Export]

The details of MX Sheet set in the Excel book are output to the CSV file.

Save destination of CSV file

After setting data export, MX Sheet saves the CSV file in the folder where the original Excel book is saved.

File name of CSV file

The following shows the file name of the CSV file.

SET*****.csv



Excel book name that executed
setting data export

Saved content of CSV file

The following shows the content of the CSV file saved by the setting data export.

Sheet Name	Use	Cell Area	Cell Area	New data	Operation	Print the	Save to	File name	Save method
J74	Logging	Logging	B2:G2	Last Line	Total	Normal	Normal		
Access	Logical S Device	Data Type	Device pr	In unit	Parzuard				
1:R16CPL D10	16bit into	1 Ward			Normal				
D100	16bit into	1 Ward							
Operation	Operation	Daily	Weekly	Monthly	Regular	Minutely	Hourly	Time Tab	Logging
Setting	Setting	Sunday			5			Log Always	
Device 1	Device 1	Device	The bit	Condition					
Setting	Setting	R0		(OH)					
Handsh	Handsh								
Setting	Setting								
CSV Log	CSV Log	No. of lin	File name	Save method					
Setting	Setting	1000	C:\ramp\	Add date and time to File name					

Automatic Save Name									
Line 1 Daily									
Automatic Save									
Setting									
Save at the end of communication									
Setting									
Set the d	Daily	Weekly	Monthly	Regular	Hourly	Time table			
Setting	Monday					17:00			
Set the D	Logical S Device	The bit	Condition	Parzuard					
Setting	1:R16CPL R1		(When OF)	Normal					
Clear cel	Specify the cell area name								
Setting	Normal								
File name	Save method								
Setting	C:\ramp\ Fix the File name								
Add dev	Logical S Device	Data Type	Value	No. of ch	Parzuard				
Setting	1:R16CPL D200	16bit into	DEC		Normal				

Automatic Print Name									
Line 1 Daily									
Automatic Print									
Setting									
Print at the end of communication									
Setting									
Set the d	Daily	Weekly	Monthly	Regular	Hourly	Time table			
Setting	Friday								
Set the D	Logical S Device	The bit	Condition	Parzuard					
Setting	Normal			Normal					
Clear cel	Specify the cell area name								
Setting	Normal								
Print Are	Sheet name to print								
Setting	Specify Sheet1								

Automatic Communication Startup									
Setting									

Displayed items

Item	Description
(1) (Cell Setting)	The settings of the sheet name and cell setting are displayed.
(2) (Automatic Save)*1	The settings of automatic save are displayed.
(3) (Automatic Print)	The settings of automatic print are displayed.
(4) (Automatic Communication Startup)	The settings of automatic communication startup are displayed.

*1 When adding device data to the saved file name, the contents of (2-1) are added at the end of <Automatic Save>.

15 SAMPLE PROGRAMS

This chapter explains the sample programs registered at MX Sheet installation.

Precautions

- The sample programs are stored in (installation folder)\Sheet\Sample at the installation. When executing the sample programs, copy them to any folder before using.
- Sample programs are provided as a reference for creating user application programs. Use the programs with your responsibility.

Logical station number

"1" is assigned to all sample programs as logical station number by default.


To use the sample programs, set the settings for the logical station number "1" or assign other logical station number and set the setting for the number.

Sample program list


The following table shows the sample programs (Sample1.xlsm, Sample2.xlsm) that are registered under (installation folder)\Sheet\Sample at MX Sheet installation.

Sample Program		Description
Excel book name	Excel spreadsheet name	
Sample1.xlsm	Logging	Logging is performed for D0 to D4 at 1 second intervals.
	Monitor, Comment, Write	Monitor, display their assigned comments and write the device data. D10 to D12 at intervals of 5 seconds.
	Alarm Summary	Alarm summary is performed using M0 to M4.
Sample2.xlsm	Monitor, Write (Conditioning)	Monitor and write the device data using device trigger.
	Logging (Conditioning)	Logging is performed using handshake.
	Automatic save	Save the data on the Excel spreadsheet automatically when M20 turns ON. (Automatic save is described in Excel spreadsheet.)


Logging sheet

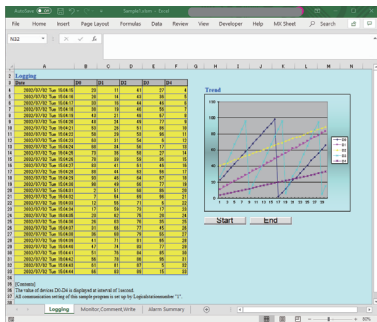


Monitor, Comment, Write sheet

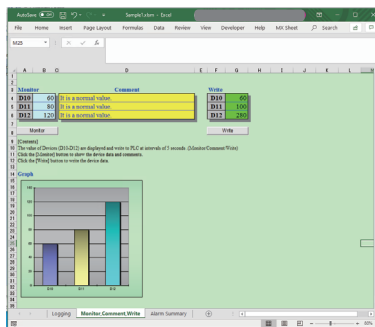


Alarm Summary sheet

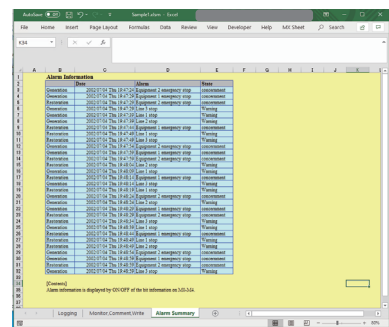


Monitor, Write (Conditioning) sheet

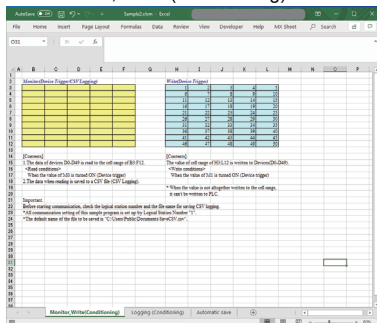

Logging (Conditioning) sheet

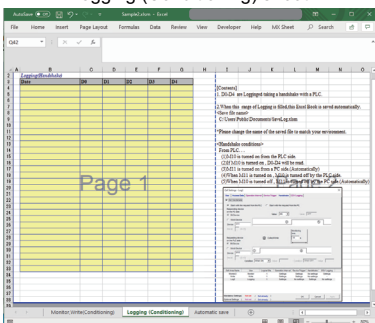

Automatic save sheet

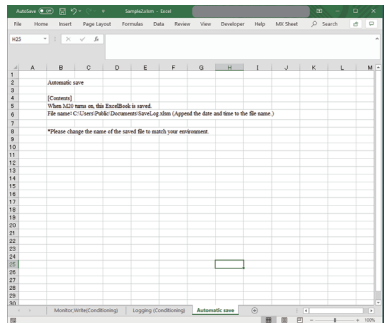

MEMO

APPENDIX

Appendix 1 Additions and Changes from Previous Version

This section shows the additions and changes with upgrade.

Additionally, the table also shows the version of MX Component that is supported by each version of MX Sheet.

MX Sheet	Description	Supported MX Component
3.000A	Microsoft Excel 2019 (32-bit version/64-bit version) is supported.	5.000A
	The supported Excel version is only Microsoft Excel 2019.	
	The supported operating system is only Windows10.	
	The default installation folder is changed from "C:\MELSEC" to "C:\Program Files\MELSOFT."	
	Available for e-Manual Viewer	
3.001B	The operability for editing a table format cell is improved.	5.002C
3.002C	Microsoft Excel for Microsoft 365 (64-bit version) is supported.	5.002C
	Menu is displayed in the ribbon format.	
3.004E	Microsoft Windows 11 is supported.	5.003D
	Microsoft Excel 2021 (32-bit version/64-bit version) is supported.	
	The number of rows that can be set for the cell area of the logging function is extended to 1000000.	
3.005F	Microsoft Windows 10 IoT Enterprise 2019 LTSC is supported.	5.004E
3.007H	The display for the number of set devices on the [Access Data] tab is improved.	5.007H

Appendix 2 Processing Speed of MX Sheet

Performance values

This section explains the performance values when the monitor and logging functions is executed using the personal computer of the following performance.

The performance values indicate the numbers of device points where no collection delay occurs when only one cell area is set to the Excel book and the device data of D device are collected by the monitor or logging function. (If multiple cell areas is set, reduce the number of device points per cell to maintain the same performance.)

The actual performance values vary depending on the performance or similar of the personal computer.

Use the performance values explained in this section as reference values.

Item		Description
Personal computer	OS	Windows 10 Enterprise (64bit)
	CPU	Intel Core i5-4590 (3.30GHz)
	Memory	16 GB
Excel		Microsoft Excel 2019 (64bit)
Cell Area		Only one

Performance values for Ethernet communication

The following table shows the performance values when the monitor and logging functions are executed using Ethernet communication.

CPU type: R08CPU

Connected module: RJ71EN71

Function	Operation Interval	Number of Device Points ^{*1}
Monitor function	0.005s (5ms)	7 points
	0.05s (50ms)	70 points
	0.5s (500ms)	900 points
	1s	1700 points
	5s	2000 points
Logging function	0.005s (5ms)	6 points
	0.05s (50ms)	60 points
	0.5s (500ms)	256 points
	1s	256 points
	5s	256 points

*1 This number of device points applies to the case the data type is set to a character string.

Number of processable device points when using system labels

This section shows the performance values (the number of processable device points) when executing the monitor and logging functions by using a personal computer with the following performance.

The actual performance values vary depending on the performance or similar of the personal computer.

Use the performance values explained in this section as reference values.

Item		Description
Personal computer	OS	Windows 10 Enterprise (64bit)
	CPU	Intel Core i5-4590 (3.30GHz)
	Memory	16 GB
Target CPU		R120PCPU (Connecting personal computer and target CPU on 1:1 basis)
Cell Area		Only one

• Setting example 1

The setting example 1 shows the case where only one access data is set.

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit	▲
1	SBL100	16bit integer	DEC		1	1	1	Word	
2									
3									

• Setting example 2

The setting example 2 shows the case where two or more units of access data are set.

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit	▲
1	SBL100	16bit integer	DEC		1	1	1	Word	
2	SBL101	16bit integer	DEC		1	1	1	Word	
3	SBL102	16bit integer	DEC		1	1	1	Word	



Only one cell can be specified with a system label on the [Access Data] tab in the cell settings screen. Up to 256 cells can be specified for the logging function.

Performance values for Ethernet communication

The following table shows the performance values when the monitor and logging functions are executed using Ethernet communication.

Function	Operation Interval	Number of Device Points*1	
		Setting example 1	Setting example 2
Monitor function	0.005s (5ms)	Collection delay occurs	Collection delay occurs
	0.05s (50ms)	1 point	60 points
	0.5s (500ms)	1 point	600 points
	1s	1 point	1300 points
	5s	1 point	2000 points
Logging function	0.005s (5ms)	Collection delay occurs	Collection delay occurs
	0.05s (50ms)	1 point	50 points
	0.5s (500ms)	1 point	256 points
	1s	1 point	256 points
	5s	1 point	256 points

*1 This number of device points applies to the case the data type is set to a character string.

Appendix 3 Processing MX Sheet

This section explains the processing of MX Sheet.

Collection delay and data dropout

On MX Sheet, collection delay, data dropout or similar problem may occur depending on the communication time with the a CPU module and the collection timing of device data.

The following explains the collection delay and data dropout.

Collection delay

Device data collection delay occurs depending on the communication time with a CPU module and the corresponding processing time.

Collection delay occurs only when "Operation time" is set to "Regular interval".

When a collection delay occurs, it is registered to the "ErrorLog" sheet as error information.


The following explains the cases where a collection delay occurs.

■When the actual communication time is longer than the specified operation interval

When the communication time with a CPU module is longer than the operation interval of MX Sheet, a device data collection delay occurs.

Ex.

"Operation time" is set to "Regular interval (3s)" but the communication time with a CPU module is 5s

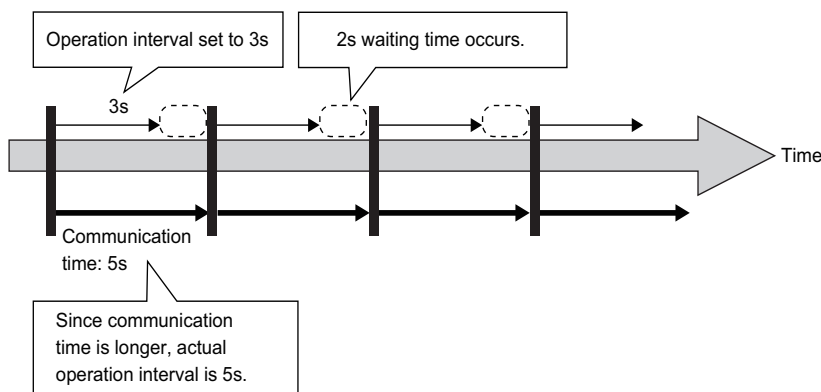


A

■Collection delay when device trigger function is used

When the sum of the device trigger condition check time and the communication time with a CPU module is longer than the operation interval of MX Sheet, a collection delay occurs during the next device trigger condition check.

Ex.

When "B0" = "When ON" is set as the device trigger condition (operation interval is 3s)

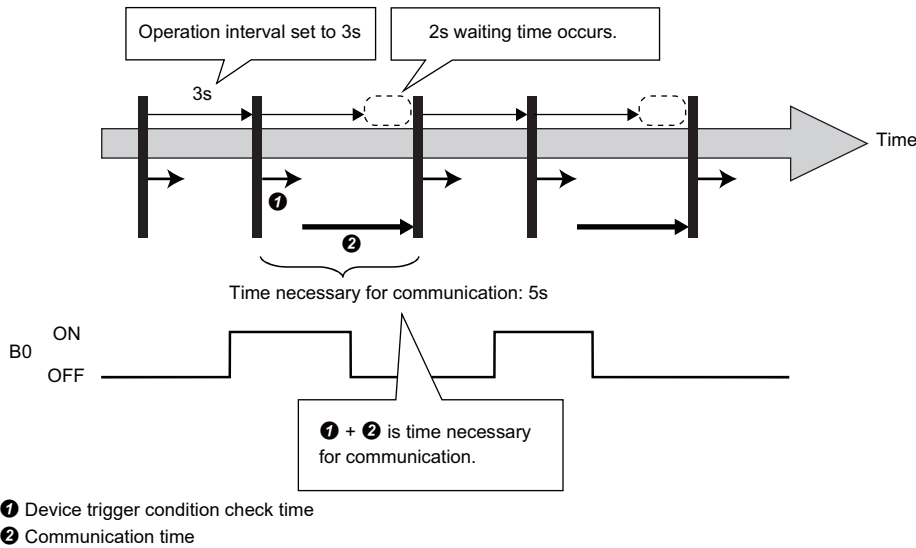


■Collection delay when handshake function is used

When the sum of the requesting device check time, the communication time with a CPU module and the handshake processing time is longer than the operation interval of MX Sheet, a collection delay occurs during the next requesting device check.

Ex.

When the "programmable controller side requesting device" is set to "M0" and the "PC side responding device" to "M100" (operation interval is 3s)

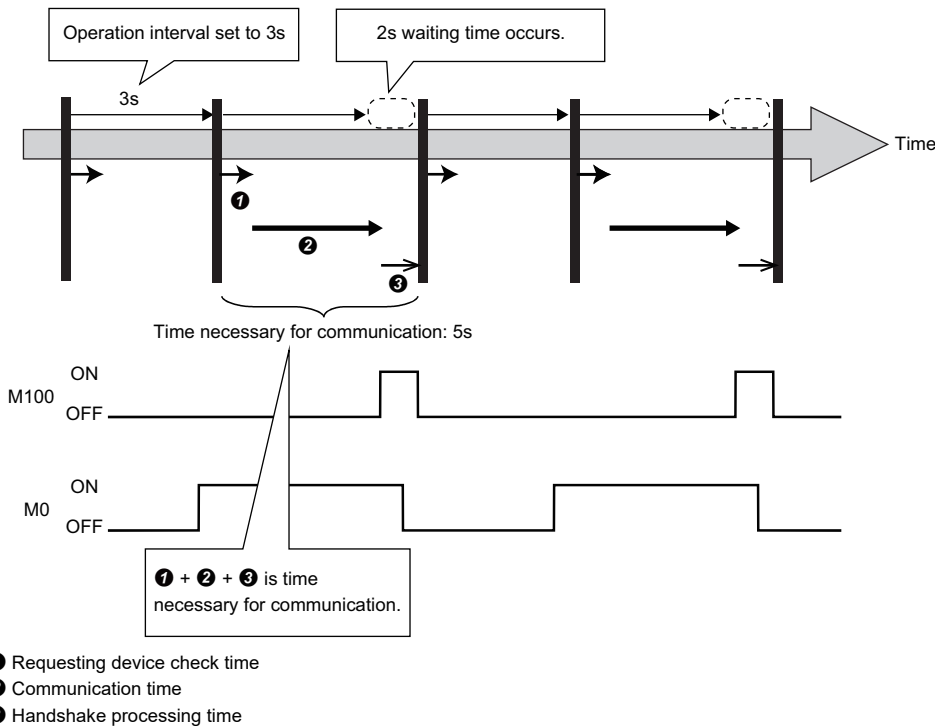

Data dropout

The data to be collected may dropout depending on the communication time with a CPU module and the collection timing of device data.

The following explains the cases where a data dropout occurs.

■When the actual communication time is longer than the specified operation interval


When the communication time with a CPU module is longer than the operation interval, the data to be collected dropouts.

If a data dropout has occurred, increase the operation interval setting of MX Sheet.

Ex.

When "Operation time" is set to "Hourly (0min, 1min, 2min)" but the communication time with a CPU module is longer than 1min

If previous data collection is still being executed when it is reached the operation time as shown below, a data dropout occurs on MX Sheet.

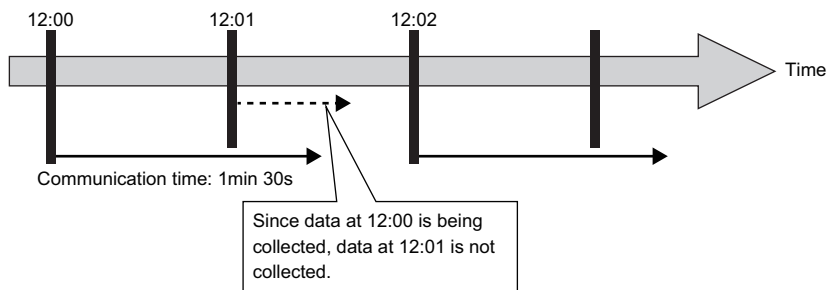

■Data dropout when device trigger function is used


When the device trigger condition holds for the specified operation time, condition cannot be checked and the data to be collected dropouts.

If a data dropout occurs during use of the device trigger, decrease the operation interval setting of MX Sheet.

Ex.

When "B0" = "When ON" is set as the device trigger condition (operation interval is 60s)

If the device trigger condition holds for the specified operation time as shown below, a data dropout occurs on MX Sheet.

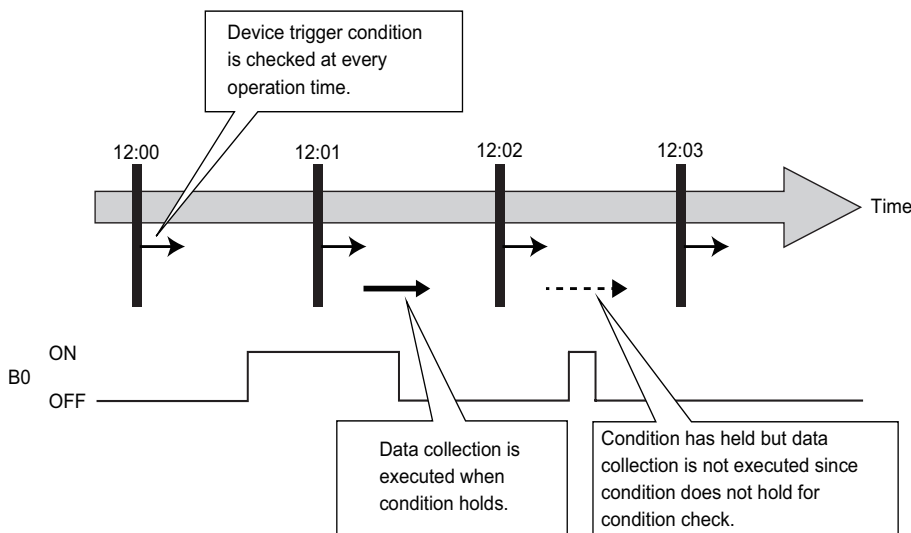

Precautions

Note that if a data dropout occurs during use of the device trigger, error information is not displayed on the "ErrorLog" sheet.


■Data dropout when handshake function is used

When the requesting device condition holds for the specified operation time, the data to be collected dropouts.
If a data dropout occurs during use of the handshake, decrease the operation interval setting of MX Sheet.

Ex.

When the "programmable controller side requesting device" is set to "M0" and the "PC side responding device" to "M100" (operation interval is 60s)

If the requesting device condition holds for the operation time as shown below, a data dropout occurs on MX Sheet.

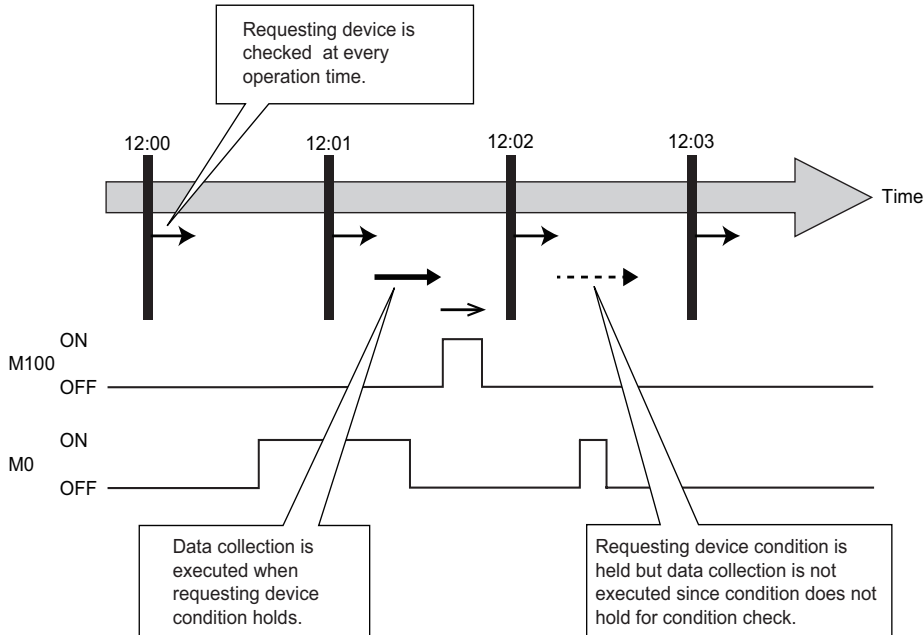

Precautions

Note that if a data dropout occurs during use of the handshake, error information is not displayed on the "ErrorLog" sheet.

Logging function

Date and time

When the logging function and CSV logging are used, the date and time in the cell area and the CSV file may not be displayed correctly.

The following explains an example of the incorrect display, the causes and corrective actions.

■Example (when "Regular interval" is set to 1s)

Although communication is performed at the specified interval, the date and time are not displayed correctly as shown below, since the time when data is actually read exceeds the regular interval.

(Error information is not displayed on the "ErrorLog" sheet because this symptom is not a collection delay.)

2022/02/11 Fri 13:08:25	32	26
2022/02/11 Fri 13:08:26	33	27
2022/02/11 Fri 13:08:28	35	27
2022/02/11 Fri 13:08:29	36	28

(1) ←

(1) Time of 13:08:28 is incorrectly displayed as 13:08:27.

- Cause

Multiple cell areas are set to the Excel book.

Multiple cell areas use the same communication route.

"Operation time" of the [Operation Interval] tab is set to "Regular interval".

- Corrective action

Decrease the number of cells set to the Excel book.

Increase the "Regular interval" setting.

Reexamine the cell area settings. (📄 Page 169 Creating the Excel Spreadsheet for MX Sheet)


Variation of logging cycle

If "Regular interval" is set in "Operation time", the logging function will operate as shown in the figure below. (For example, when a cycle is 10 seconds and communication time is 5.2 seconds, the logging function waits for the next cycle for 4.8 seconds.)

A communication time and waiting time can be calculated in an internal processing of MX Sheet using the time on Windows. Since an internal processing is affected by time deviation on Windows and the load state of a personal computer, the time between the calculated time and the actual time may differ.

Consequently, logging cycles vary.

Operation interval: 10 seconds

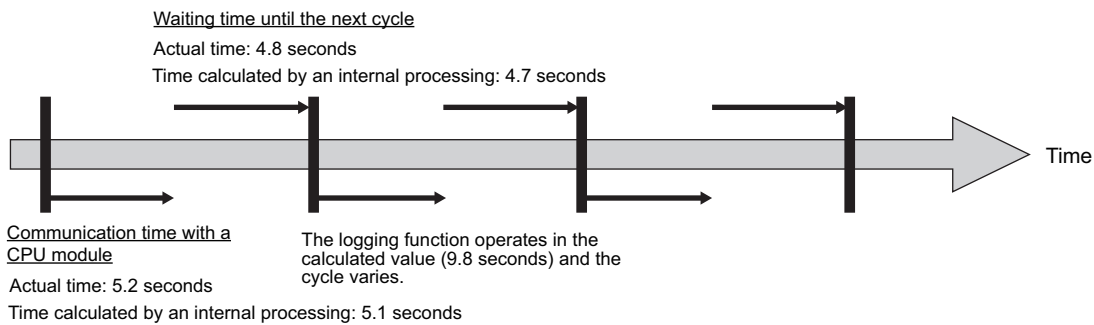

Appendix 4 Creating the Excel Spreadsheet for MX Sheet

When collecting/writing device data by using MX Sheet, the efficiency of communication with a CPU module varies depending on the cell area settings.

The following provides the example of setting cell area for more effective communication.


Communication efficiency and cell area specifying method

When multiple cell areas are set, MX Sheet executes communication with a CPU module in order of the cell areas.

When the same communication route is set to multiple cell areas, communication efficiency decreases since all cell areas use one communication route to communicate with the CPU module.

The following setting example shows the case where the same communication route is set to multiple cell areas.

- Setting example

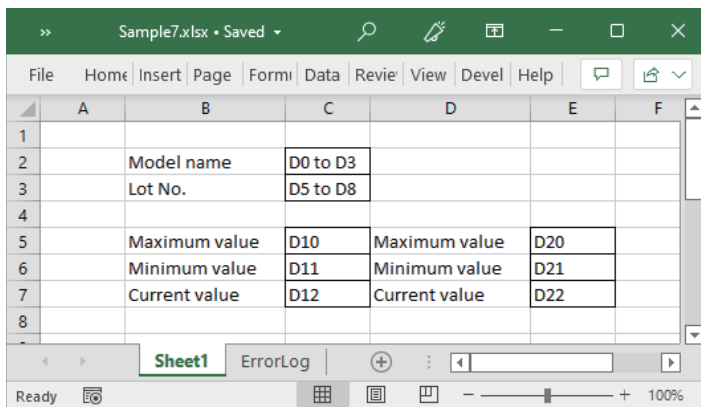

Inefficient setting

When the above setting example is divided into four cell areas as shown in the following table, MX Sheet executes communication four times. This causes communication load to increase; therefore decreases communication efficiency.

Cell area name	Cell area	Access data settings			Operation Interval
		Logical station number	Device setting	Number of cells	
Model name	C2	0: Ethernet	D0 Character string	1	1s interval
Lot No.	C3		D5 Character string		
A	C5:C7		D10 16-bit integer	3	
B	E5:E7		D20 16-bit integer		

Efficient setting

When the above setting example is integrated into one cell area as shown in the following table, the collection/writing of device data is completed by performing communication once. This enables communication load to decrease; therefore improves communication efficiency.


Cell area name	Cell area	Access data settings			Operation Interval
		Logical station number	Device setting	Number of cells	
Product information	C2,C3,C5:C7,E5:E7	0: Ethernet	D0 Character string	1	1s interval
			D5 Character string		
			D10 16-bit integer	3	
			D20 16-bit integer		

A

Communication efficiency and access data setting

When one type of device is set as multiple devices, the efficiency of communication with a CPU module. The following setting example shows the case where one type of device is specified consecutively.

- Setting example

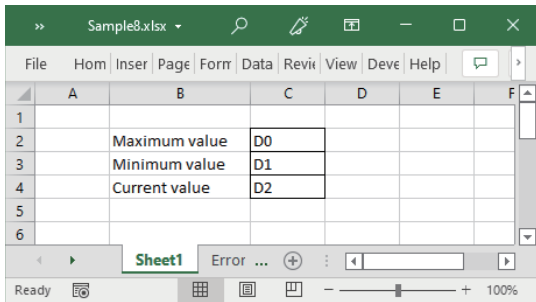

Inefficient setting

When the above setting example is divided into three access data as shown below, MX Sheet recognizes them as three types of devices and executes communication. Therefore the communication efficiency is decreased.

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	D0	16bit integer	DEC	1	1	1	1	Word
2	D1	16bit integer	DEC	1	1	1	1	Word
3	D2	16bit integer	DEC	1	1	1	1	Word

Efficient setting

When the above setting example is integrated into one access data as shown below, MX Sheet recognizes it as one type of device and executes communication. Therefore the communication efficiency can be improved.

	Device	Data Type	Value	No. of characters	Zoom	No. of cells	Dev. points	In unit
1	D0	16bit integer	DEC	1	3	3	3	Word
2								
3								

Point

Any of the following settings prevents the improvement of communication efficiency even if an efficient setting is configured.


- When "Data Type" is set to "Bit", the device number setting of "Device" is not a multiple of 16.
- CN200 (current value of 32-bit counter device) or later of the FXCPU is set.

Communication efficiency and use of Excel function (cell reference)

When inconsecutive device data is displayed on Excel, the efficiency of communication with CPU module decreases if multiple cell areas are set.

The following setting example shows the case where inconsecutive device data is displayed on Excel.

- Setting example

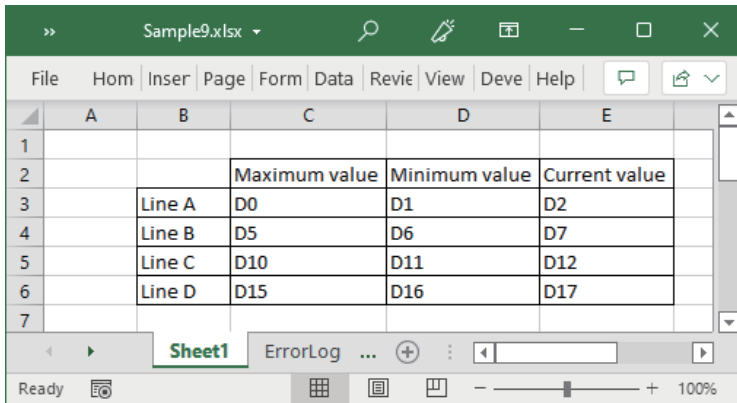

Inefficient setting

When the above setting example is divided into four cell areas as shown in the following table, MX Sheet executes communication four times. This causes communication load to increase; therefore decreases communication efficiency.

Cell area name	Cell area	Access data settings			Operation Interval
		Logical station number	Device setting	Number of cells	
Line A	C3:E3	0: Ethernet	D0 16-bit integer	3	1s interval
Line B	C4:E4		D5 16-bit integer		
Line C	C5:E5		D10 16-bit integer		
Line D	C6:E6		D15 16-bit integer		

A

Efficient setting

By integrating the above setting example into one cell area and collecting device data into the other Excel spreadsheet (Sheet2) as shown in the following table, these decrease communication load; therefore improves communication efficiency. Set cell references so that Excel spreadsheet (Sheet1) that actually displays the device data is refer to the corresponding cells within Excel spreadsheet (Sheet2) that collects the device data.

(MX Sheet need not be set in the Excel spreadsheet (Sheet1) where device data is displayed.)

Cell area name	Cell area	Access data settings			Operation Interval
		Logical station number	Device setting	Number of cells	
Line information	A2:E5 (Area set to Sheet2)	0: Ethernet	D0 16-bit integer	20	1s interval

Sheet 1 (Excel spreadsheet where device data is displayed actually)

	A	B	C	D	E	F
1			Maximum value	Minimum value	Current value	
3		Line A	=Sheet2!A2	=Sheet2!B2	=Sheet2!A3	
4		Line B	=Sheet2!A3	=Sheet2!B3	=Sheet2!A4	
5		Line C	=Sheet2!A4	=Sheet2!B4	=Sheet2!A5	
6		Line D	=Sheet2!A5	=Sheet2!B5	=Sheet2!A6	

Sheet 2 (Excel spreadsheet where device data is collected)

	A	B	C	D	E	F	G
1	Line monitor						
2	D0	D1	D2	D3	D4		
3	D5	D6	D7	D8	D9		
4	D10	D11	D12	D13	D14		
5	D15	D16	D17	D18	D19		


Set Sheet 1 to refer to cells of Sheet 2.

Appendix 5 Procedure to Transport Data to Other Personal Computer

This section explains the procedure to transport the settings of MX Sheet from a development personal computer to an on-site personal computer.

Point

MX Sheet and MX Component must be installed in the personal computer where the settings of MX Sheet is transported.

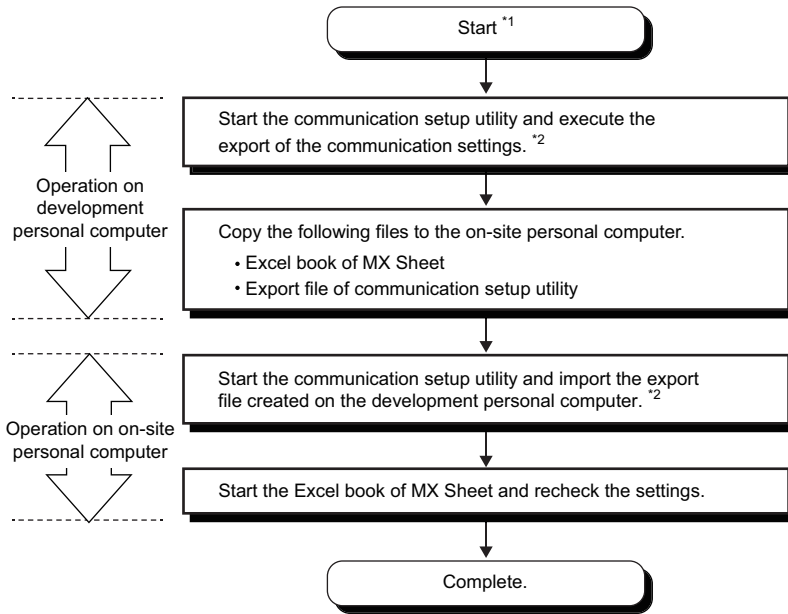

*1 The Excel book for MX Sheet should be created on the development personal computer.

*2 For the import and export operations of communication settings, refer to [MX Component Version 5 Reference Manual](#).


Appendix 6 HTML File

This section explains the HTML file saved during MX Sheet operation.

HTML file


MX Sheet allows an HTML file to be saved automatically into the folder specified when any of the following functions is used.

- Logging function (when cell is full)
- Alarm summary function (when cell is full)
- Automatic save setting

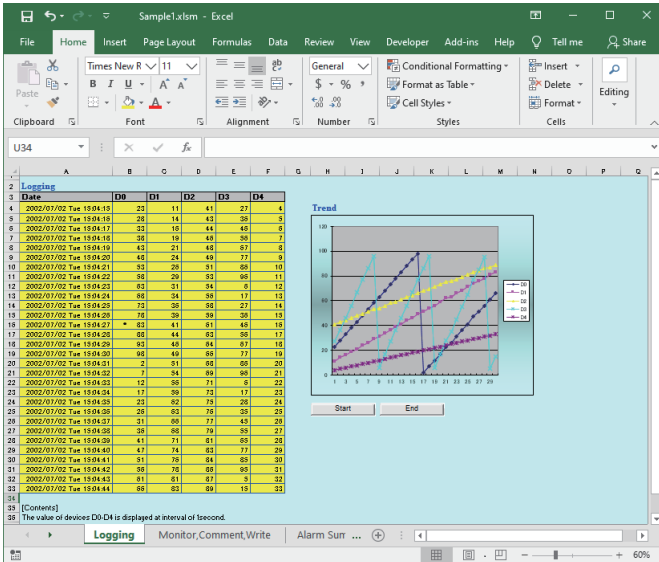

Convenient use of HTML file

The data collected by MX Sheet can be snapshot-monitored from a business destination, office or other places via the Internet/intranet, with the plant side personal computer (a personal computer where MX Sheet is operating) used as a Web server.

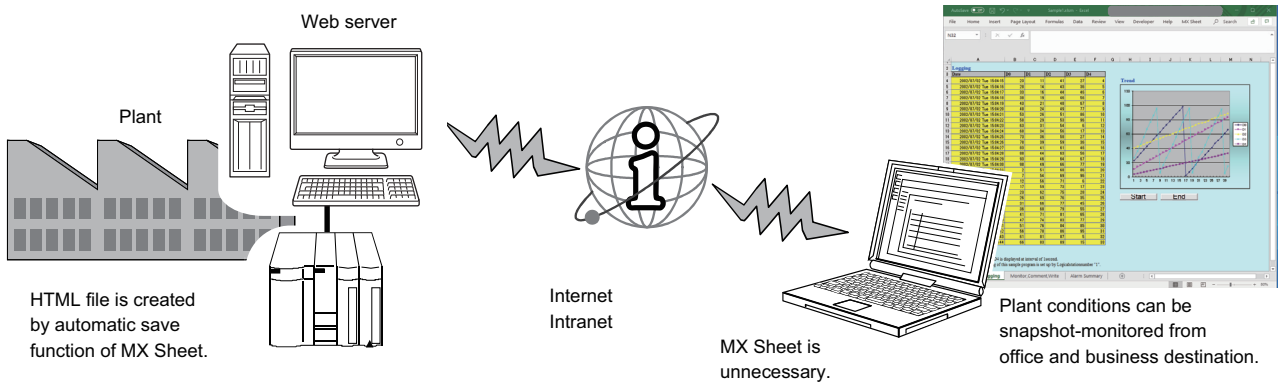

Appendix 7 CSP+ For Machine

CSP+ file for machine is a file that expresses CSP+ for machine in XML format. This section explains the CSP+ for machine that can be used for MX Sheet. For CSP+, refer to the CC-Link Partner Association website (www.cc-link.org).

Specification versions of CSP+ for machine

Specification versions of CSP+ for machine that can be used for MX Sheet are the major version 1 and 2.

DATATYPE of CSP+ for machine

The following table shows the data types of MX Sheet corresponding to those of DATATYPE of CSP+ for machine that can be used for MX Sheet.

CSP+ for machine DATATYPE	MX Sheet						
	Data type	Value	No. of characters	Zoom	Number of cells	Dev. points	In unit
BOOL	Bit	—	—	—	1	1	Bit
INT8	16 bit integer	Decimal	—	1	1	1	Word
UNIT8							
INT16							
INTx (x: 2 to 15)							
UNIT16							
UNITx (x: 2 to 15)							
WORD							
BIT_STRINGx (x: 2 to 15)							
DWORD	32 bit integer	—	—	—	1	1	Word
UNIT32							
INT32							
BYTE	16 bit integer	—	—	—	1	1	Word
STRINGx (x: 1 to 40)	Character string	—	x	—	—	x/2	Word
DATE	16 bit integer	Decimal	—	1	8	8	Word
BIN8					1	1	
BIN16					—	—	
BINx (x: 1 to 15)					—	—	
BIN32					2	2	
	32 bit integer	—	—	—	—	—	Word




ASSIGN of CSP+ for machine

The following table shows the devices of ASSIGN of CSP+ for machine that can be used for MX Sheet.

Device	Type
Special relay (SM)	Bit
Special register (SD)	Word
Input (X)	Bit
Output (Y)	Bit
Internal relay (M)	Bit
Latch relay (L)	Bit
Annunciator (F)	Bit
Edge relay (V)	Bit
Link relay (B)	Bit
Data register (D)	Word
Link register (W)	Word
Link special relay (SB)	Bit
Link special register (SW)	Word
Extension file register (ZR)	Word

Appendix 8 Warning Messages on Windows

A warning message appears by the user account control function when executing Excel as an administrator.

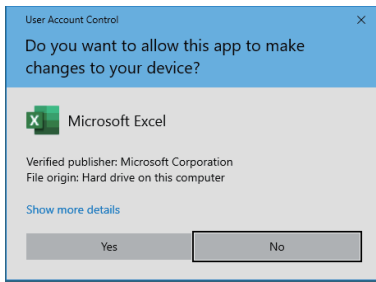

Appendix 9 Troubleshooting

Symptom	Check point	Corrective action
The following symptom occurs when upgrading the version of Excel. • "Run-time error '9' : Subscript out of range" is displayed when Excel is started up.	Does a temporary file created by Excel remain?	Delete the temporary file according to the following procedure. (☞ Page 178 Considerations for deleting a temporary file) ① Enter '%temp%\Excel8.0.' in Windows Explorer, and delete the files under '%temp%\Excel8.0.' ② Enter '%AppData%\Microsoft\Excel' in Windows Explorer, and delete the '.xlb' file under '%AppData%\Microsoft\Excel.'
The following symptom occurs when upgrading the version of MX Sheet. • After setting the automatic communication startup setting in MX Sheet, the available/unavailable buttons for the function are inappropriate.	Does a temporary file created by Excel remain?	Delete the temporary file according to the following procedure. (☞ Page 178 Considerations for deleting a temporary file) ① Enter '%temp%\Excel8.0.' in Windows Explorer, and delete the files under '%temp%\Excel8.0.' ② Enter '%AppData%\Microsoft\Excel' in Windows Explorer, and delete the '.xlb' file under '%AppData%\Microsoft\Excel.'
Data is not written to a programmable controller after starting the communication.	Has the following error occurred in an "ErrorLog" sheet? • The wrong value is inputted into the cell area. Write process of the corresponding cell area was not performed.	<ul style="list-style-type: none"> • If there is no data for the number of device points specified in the [Access Data] tab in the cell area specified in the "Cell Settings" screen, review the setting. • Set the data which matches to the data type specified in the [Access Data] tab. <ul style="list-style-type: none"> ① For bit type: Either 0 or 1 ② For integer/real number type: Numeric data (other than character string) • If "zoom" has set, set the data so that the operation result does not overflow.
An communication error occurs during communication with a CPU module.	Is any of the following functions set to a personal computer on which MX Sheet is installed? • Resume function • Suspend function • Power saving function • Standby mode	Do not set any of the following functions on the personal computer. <ul style="list-style-type: none"> • Resume function • Suspend function • Power saving function • Standby mode
The "Operation of Excel sheet failed." message is displayed when selecting [Cell Setting] in the [MX Sheet] tab.	<ul style="list-style-type: none"> • Has MX Component been installed? • Is the sheet name changed by the operation of Excel? 	<ul style="list-style-type: none"> • When MX Component has not been installed, install it. • When the sheet name is changed by the operation of Excel, restore the sheet name. Change the sheet name from the menu of MX Sheet. <p>When the symptom cannot be solved by the above actions, take the following actions:</p> <ul style="list-style-type: none"> • Enable the ActiveX setting and the macro setting in the security setting of Excel. (☞ Page 22 Security settings of Excel) • Start Excel from the [Run as administrator] menu.
The message "The selected cell area is set already." is displayed at the time of cell setting.	Is the operation procedure for setting a cell correct?	Set the cell by the following procedure. ① Select a cell of an Excel spread sheet on which the cell is not set. ② Select [Cell Setting] in the [MX Sheet] tab. ③ Select a cell area to be edited from the cell area list on the "Cell Settings" screen.
When MX Sheet setting is set, only the frame of Excel is displayed.	Is the operation of logging off or shutting down of a personal computer performed during communication?	Remove the hidden attributes of the Excel book and overwrite the Excel book to restore the system by the following procedures. ① Select the [View] tab and select [Unhide]. ② Select the Excel book to be displayed and click the [OK] button. ③ As the Excel book is displayed, save the Excel book.
The timeout error (0x0180840B) occurs during communication.	—	Recover from the error by the following corrective actions. <ul style="list-style-type: none"> • Check the CPU module, unit settings, state of the cable, etc. • Check if communication can be established with the Ping command. • Review the timeout time of Communication Settings Utility. • Review the timeout time of the property of the control.

Symptom	Check point	Corrective action
The socket object generation error (0x01808007) occurs during communication.	Is GT SoftGOT used?	When using GT SoftGOT, right-click and select "Run as administrator" at the startup of the application. When the symptom cannot be solved by the above action, set a port number different from one used for another application to the personal computer side. If the symptom cannot be solved, check the following items, and contact your local Mitsubishi Electric sales office or representative. <ul style="list-style-type: none"> • System configuration (model name of the target programmable controller, model name of the module, and used network) • Name of personal computer (Manufacturer), CPU, memory size • OS, Edition, 32-bit/64-bit • MX Component version • A function and argument of MX Component in which the symptom occurs • Settings within "Communication Settings Utility" • Occurrence frequency and procedure for a symptom
The start communication button cannot be moved.	Is the operation procedure of Excel correct?	Operate Excel by the following procedures. <ol style="list-style-type: none"> 1 Select [Design Mode] in the [Developer] tab to enter the design mode. 2 Select the start communication button and drag it.
Any of the following messages appears. <ul style="list-style-type: none"> • Acquisition of Excel sheet Information failed. • Operation of Excel sheet failed. 	Does MX Component support the connection target device that MX Sheet supports? Is there any problem with the Excel file location?	Use MX Component that supports the connection target device that MX Sheet supports. Open the Excel file to be used in MX Sheet from a local folder. If the file is synchronized with OneDrive, etc., disable the synchronization.
An error message appears for the device specified on the [Access Data] tab.	Is the communication route of the logical station number assigned to the cell area supported by MX Sheet?	Use the logical station number which is supported by MX Sheet.
The following message appears on the "ErrorLog" sheet at the start of communication. <ul style="list-style-type: none"> • Communication error has occurred in the open/close of communication. 	<ul style="list-style-type: none"> • Is the logical station number supported by MX Component used? • Has the communication route been changed to the one, which is not supported by MX Sheet after a logical number is assigned in MX Sheet? 	<ul style="list-style-type: none"> • Use the logical station number which is supported by MX Component. • Use the logical station number which is supported by MX Sheet.
<ul style="list-style-type: none"> • Excel stops responding. • System error in MXShComnInitialize or the following message appears: Can't execute code in break mode. 	<ul style="list-style-type: none"> • Is an Excel book where the MX Sheet automatic communication startup setting is set opened? • Is an Excel book opened with Microsoft Excel 2007 or later? 	Perform the operation described in the "Corrective action" in the following: <ul style="list-style-type: none"> ☞ Page 179 Countermeasures for errors as a result of setting the automatic communication startup setting in an Excel book and opening it in Microsoft Excel 2007 or later

Considerations for deleting a temporary file

Check the following before deleting the temporary file:

- A folder differs for each logon user. Take an action for each logon user to be used.
- Display all files and folders to take an action by the following procedures:
 - 1 Click the [View] tab in Windows Explorer, and select [Options].
 - 2 Click the [View] tab, and select "Show hidden files, folders, and drives" in the [Advanced settings] box.
- A file and folder may not exist.

Point


When "Display error log" is selected on the [Error log] tab on the "Options" screen (☞ Page 152 Setting Error Logs), errors occurred on MX Sheet are output to the "ErrorLog" sheet.

For the method for checking the error codes output on the "ErrorLog" sheet, refer to the following:

☞ Page 155 Checking method for the error codes output on an "ErrorLog" sheet

Countermeasures for errors as a result of setting the automatic communication startup setting in an Excel book and opening it in Microsoft Excel 2007 or later

When opening an Excel book where the automatic communication startup setting (☞ Page 129 AUTOMATIC COMMUNICATION STARTUP/CANCELLATION) is set in Microsoft Excel 2007 or later, Excel may not respond and any of the following messages may appear.

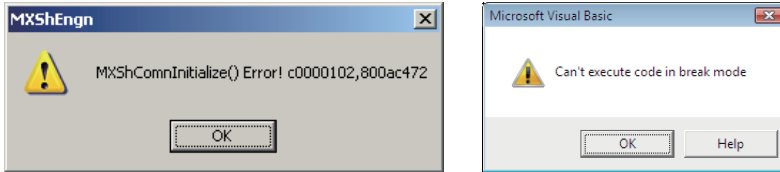

Corrective action

Take an action by the following procedures:

1. Check the required .NET Framework and the related modules, and install them. (☞ Page 179 Checking and installation of .NET Framework and the related module)
2. Execute "MXShRegRCom.exe." (☞ Page 180 Execution of "MXShRegRCom.exe")
3. Check if the action works. (☞ Page 181 Checking if the action works)

Point

Update MX Sheet or install Service Pack, .NET Framework, and the related module using the administrator account.

Checking and installation of .NET Framework and the related module

The following tables list .NET Frameworks and the related module required for each operating environment.

If they are not installed, install them in the order listed in the table.

The file is in the "DOTNET" folder.

■When using Windows 11 and Windows 10

".NET Framework 4.8 Advanced Services" or ".NET Framework 4.6 Advanced Services" needs to be enabled in "Turn Windows features on or off" on the control panel.

- 32-bit version

Excel version	.NET Framework and the related module	Name of file in product DVD
Microsoft Excel 2021 Microsoft Excel 2019	Microsoft .NET Framework 4.6 Extended	dotNetFx40_Full_x86_x64.exe
	Microsoft Visual Studio 2010 Tools for Office Runtime (x86)	vstor_redist.exe

- 64-bit version

Excel version	.NET Framework and the related module	Name of file in product DVD
Microsoft Excel 2021 Microsoft Excel 2019	Microsoft .NET Framework 4.6 Extended	dotNetFx40_Full_x86_x64.exe
	Microsoft Visual Studio 2010 Tools for Office Runtime (x64)	vstor_redist.exe

Point

Check if the required .NET Framework and the related module are installed or not by the following operations. [Uninstall a program] in the control panel of Windows

Check if the "Uninstall or a change a program" screen displays the required .NET Framework and the related module.


Execution of "MXShRegRCom.exe"

After installing .NET Framework and the related module, execute "MXShRegRCom.exe" in the folder where MX Sheet is installed (any of the following folders when the installation folder was not changed at installation).

- 32-bit version operating system: C:\Program Files\MELSOFT\Sheet
- 64-bit version operating system: C:\Program Files (x86) \MELSOFT\Sheet


When the user account control is enabled, the following screen is displayed.

Click the [Yes] button.

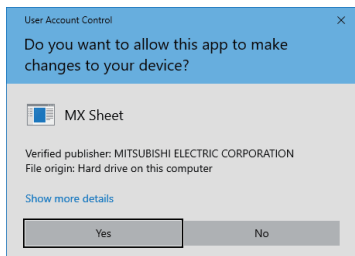

The following message is displayed to notify the completion.





Click the [OK] button.

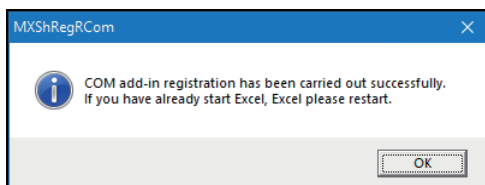

Checking if the action works

The following explains how to check if the action works or not.

1. Start Excel.
2. When the screens on the left appear, click the [Install] button.

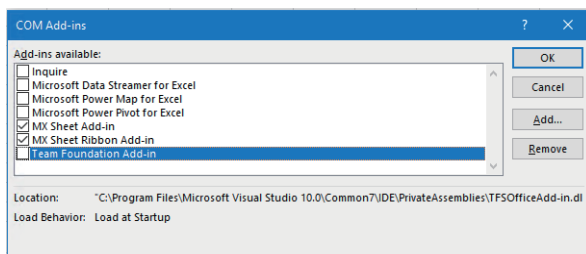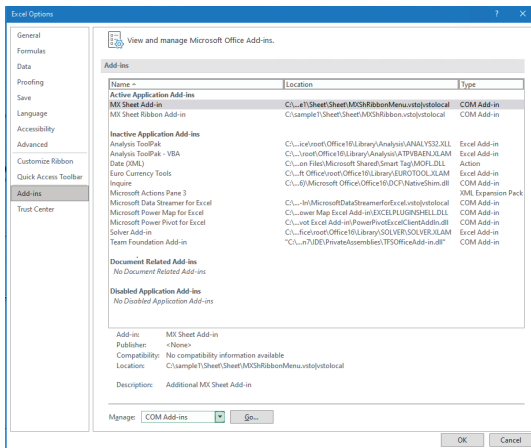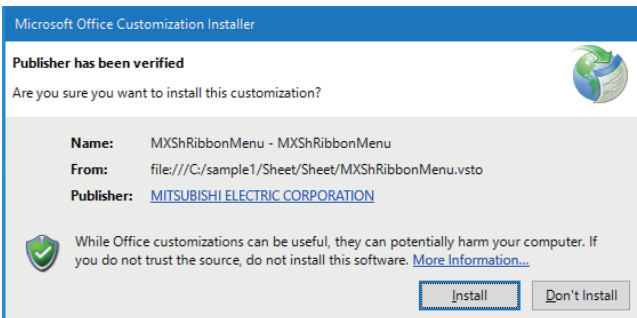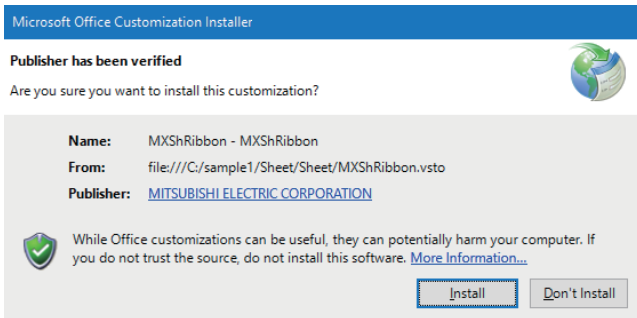

3. Select the [File] tab ⇒ [Options]. The "Excel Options" screen is displayed.
4. Select "Add-Ins," change the item in "Manage" to "COM Add-ins," and click the [Go] button.
5. "MX Sheet Ribbon Add-in" is displayed in the "COM Add-Ins" screen. Check that the checkbox of "MX Sheet Ribbon Add-in" is selected.

A


Countermeasures when MX Sheet add-ins remain in the EXCEL add-in list

Add-ins are changed from EXCEL add-ins to COM add-ins in MX Sheet Ver3.002C.


Therefore, when updating MX Sheet from Ver.3.001B or earlier to Ver3.002C or later, MX Sheet add-ins may remain in the EXCEL add-in list.

Delete MX Sheet add-ins by the following procedure:


1. Delete the following files if they remain in the installation destination folder of MX Sheet (the "C:\Program Files (x86)\MELSOFT\Sheet" folder as default).
 - MXShMenu.xlam
 - MXShRibbon.xlam
 - MXShMenu.xla
2. Select "Mxshmenu" ("MX Sheet") from EXCEL add-ins. If it does not exist, proceed to the step 4.

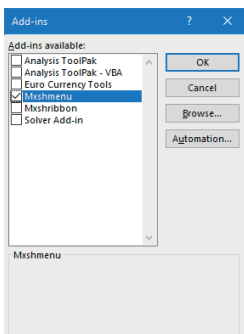


3. The following message appears. Click the [Yes] button.

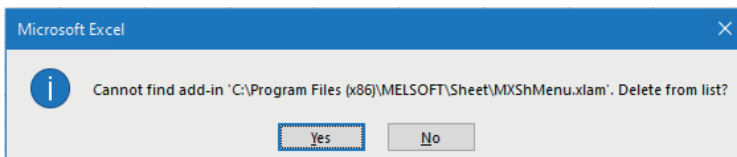

4. Select "MXshribbon" ("Additional MX Sheet Add-in") from EXCEL add-ins. If it does not exist, further steps are not required.

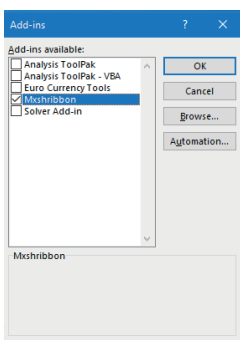

5. The following message appears. Click the [Yes] button.

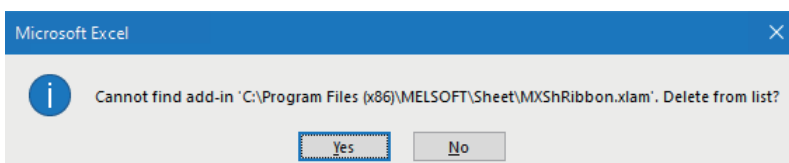

Appendix 10 Useful Functions


Alarm summary

Alarm summary converts ON/OFF data of bit devices into alarm comment character strings that are set separately and accumulates them on an Excel spreadsheet as alarm history.

When the number of alarm histories reaches to the last row, the following operations can be specified:

- Scrolling
- Printing an Excel spreadsheet
- Saving an Excel Book

By accumulating the alarm history, status such as the operation rate of production line can be checked easily.

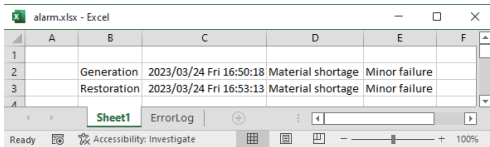


	A	B	C	D	E	F
1						
2		Generation	2023/03/24 Fri 16:50:18	Material shortage	Minor failure	
3		Restoration	2023/03/24 Fri 16:53:13	Material shortage	Minor failure	

Alarm data is accumulated as bit devices turn ON/OFF.

Comment display


Comment display converts bit or device values into comment character strings that are set separately and displays them on an Excel spreadsheet. (The comment is displayed according to the change of the device value.)

For example, the upper and lower limit values is set in a device, and when the device values becomes out of the range, a warning message appears.

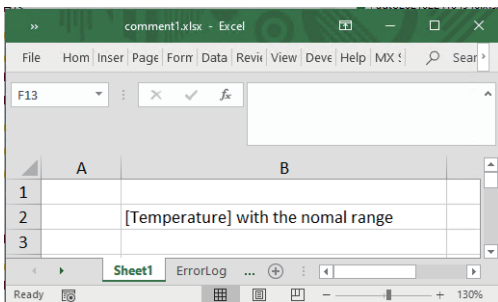

	A	B
1		
2		[Temperature] with the normal range
3		

Temperature rise

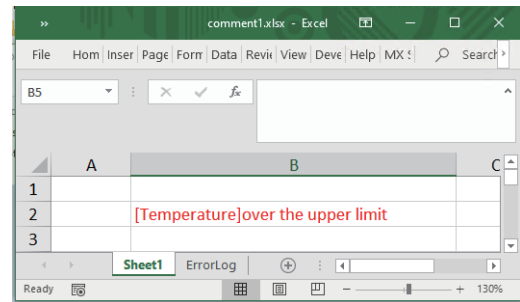


	A	B	C
1			
2		[Temperature] over the upper limit	
3			

A

Device trigger

Device trigger sets device conditions for collecting/writing the device data, and collects/writes device data when the set device conditions are met.

- When the device data is collected/written while bit device is ON

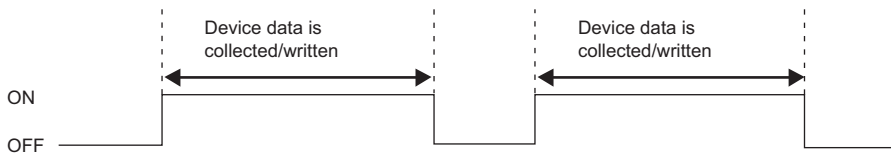

■Corresponding functions


- Logging
- Monitor
- Write
- Alarm summary
- Comment display
- Automatic save
- Automatic print

Handshake


Handshake sets handshake with a CPU module for secure device data collection/write.

Handshake checks whether data transferring can be performed by exchanging the signal of sending request and receiving reply between a personal computer and a programmable controller at data updating, and sends data if it is possible.

- When starting with the request from the PLC

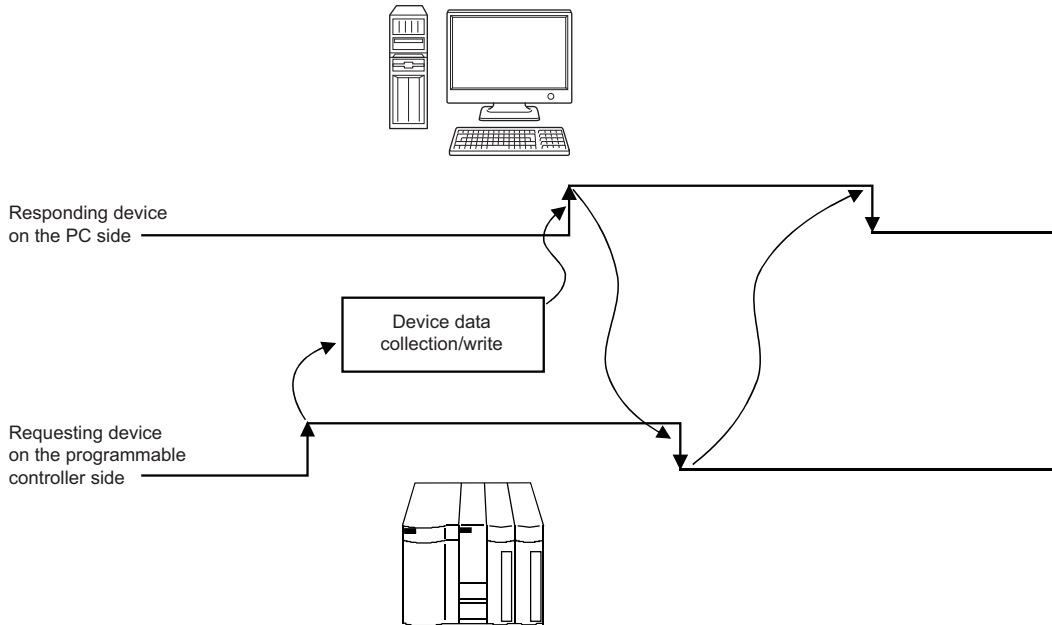


- When starting with the request from the PC

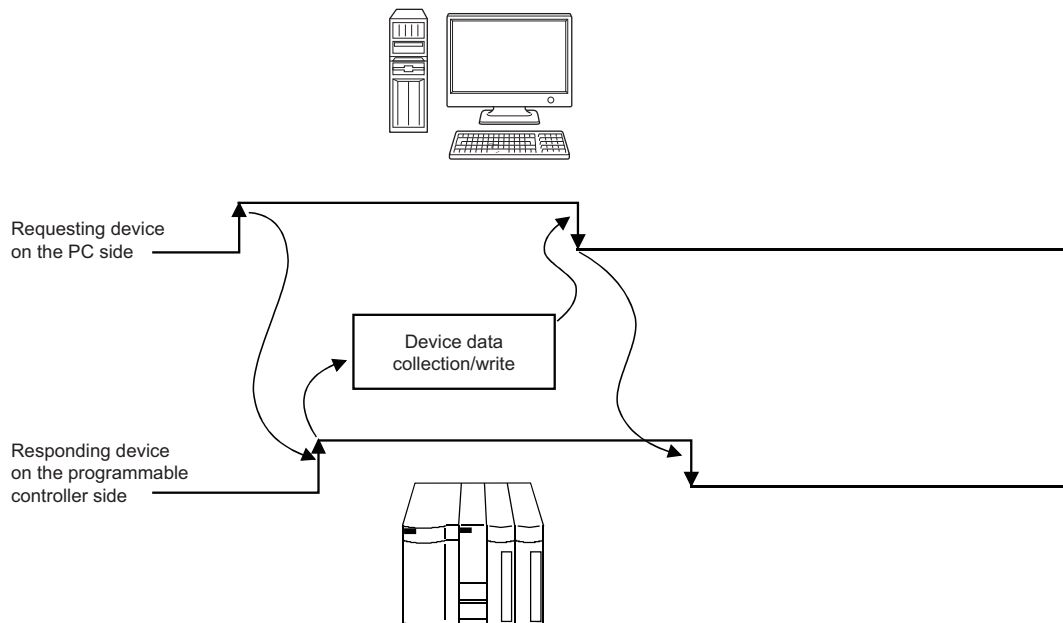

CSV logging

CSV logging displays device data on an Excel spreadsheet with logging or monitor function, and simultaneously saves collected data as a CSV file.

Long-term data collection is available with a single CSV file.

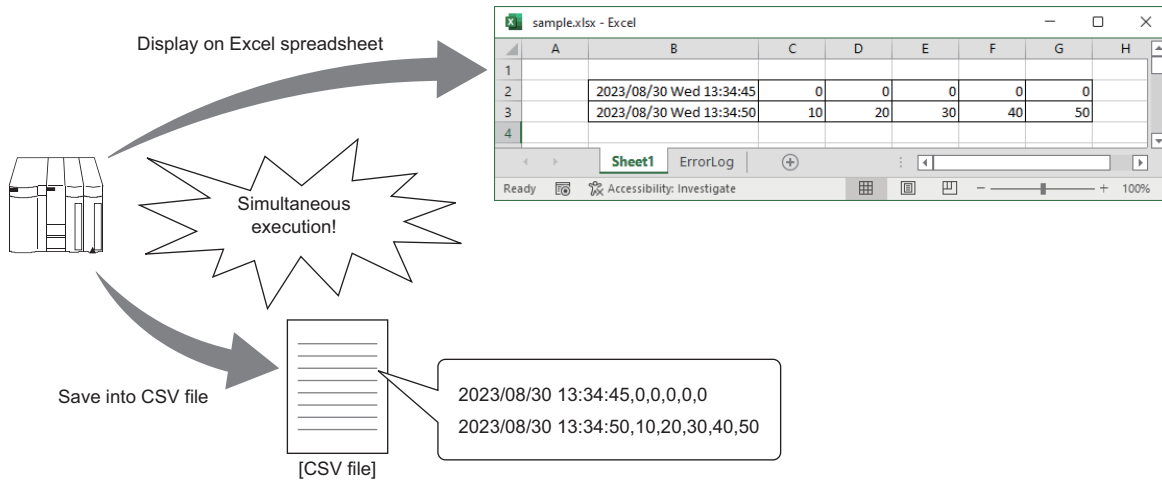

Automatic communication startup


This is a setting to start communication with a programmable controller automatically when starting an Excel book where MX Sheet settings are set.

Selecting [Start] from the MX Sheet menu is not required.

Protecting MX Sheet setting

MX Sheet settings is protected with a password.

Changing the content set by a user is prevented.

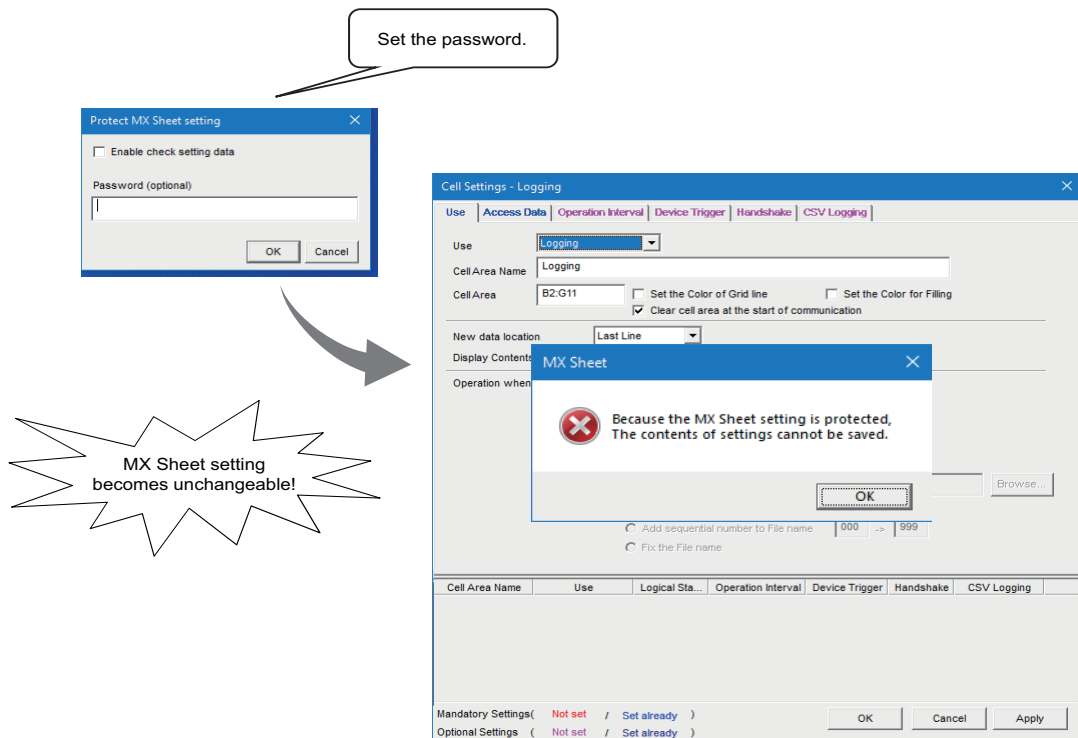

Setting error logs

When starting the communication, an "ErrorLog" sheet which shows the communication status of MX Sheet is created, and the communication status, error information, and corrective action are output.

The following error log settings can be set to this "ErrorLog" sheet in the option setting.

Type setting of error logs to be output

The types of error log to be output (information, error, warning) can be specified.


Ex.

When outputting all the error logs

Kind	Date	Cell Area Name	ErrorNo	Contents
Error	2022/02/17 Thu 12:40:05	logging	e1000009	The specified logical station number is not set. The corrective action is as follows: Create the logical station number after performing communication setting.
Information	2022/02/17 Thu 12:43:08		00000002	Communication was completed.

Automatic display switching setting of "ErrorLog" sheet

An "ErrorLog" sheet can be switched and displayed automatically when an error occurs.

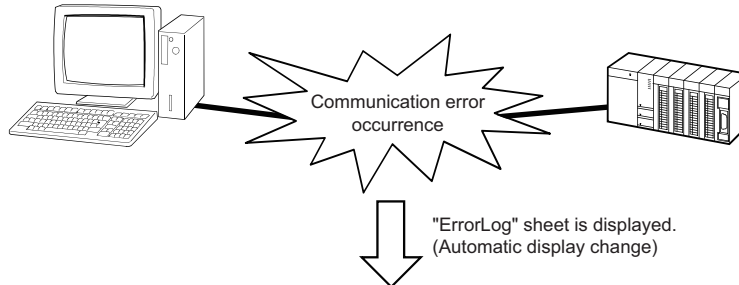

Kind	Date	Cell Area Name	ErrorNo	Contents
Error	2022/02/17 Thu 12:40:05	logging	e1000009	The specified logical station number is not set. The corrective action is as follows: Create the logical station number after performing communication setting.
Information	2022/02/17 Thu 12:43:08		00000002	Communication was completed.

Error log clearing setting at communication start

The error log can be cleared at the start of communication.

A

Appendix 11 Compatibility With Existing Products



Comparison with MX Sheet Version 2

This section explains the differences between MX Sheet Version 2 and Version 3.

■ Operating environment (Applicable software)

	MX Sheet Version 2	MX Sheet Version 3
Operating system ^{*1}	Microsoft Windows XP Professional Microsoft Windows XP Home Edition Microsoft Windows Vista Home Basic Microsoft Windows Vista Home Premium Microsoft Windows Vista Business Microsoft Windows Vista Ultimate Microsoft Windows Vista Enterprise Microsoft Windows 7 Starter Microsoft Windows 7 Home Premium Microsoft Windows 7 Professional Microsoft Windows 7 Ultimate Microsoft Windows 7 Enterprise Microsoft Windows 8 Microsoft Windows 8 Pro Microsoft Windows 8 Enterprise Microsoft Windows 8.1 Microsoft Windows 8.1 Pro Microsoft Windows 8.1 Enterprise Microsoft Windows 10 Home Microsoft Windows 10 Pro Microsoft Windows 10 Enterprise Microsoft Windows 10 Education	Microsoft Windows 10 Home Microsoft Windows 10 Pro Microsoft Windows 10 Enterprise Microsoft Windows 10 Education Windows 10 IoT Enterprise 2016 LTSC Windows 10 IoT Enterprise 2019 LTSC Microsoft Windows 11 Home Microsoft Windows 11 Pro Microsoft Windows 11 Enterprise Microsoft Windows 11 Education
Excel ^{*1}	Microsoft Excel 2003 (English version) Microsoft Excel 2007 (English version) ^{*1} Microsoft Excel 2010 (English version) ^{*1} Microsoft Excel 2013 (English version) ^{*1} Microsoft Excel 2016 (English version) ^{*1} Microsoft Excel 2019 (English version)	Microsoft Excel 2019 (English version) Microsoft Excel 2021 (English version) Microsoft Excel for Microsoft 365 (64-bit version) (English)

*1 For the restrictions for each operating system and Excel version, refer to the following:

- MX Sheet Version 2:  MX Sheet Version 2 Operating Manual
- MX Sheet Version 3:  MX Sheet Version 3 Installation Instructions

Point

- Using the unsupported operating environment
Use MX Sheet Version 2 when using the operating environment which is not supported by MX Sheet Version 3.

Compatibility

■ Installation

MX Sheet Version 3 cannot be installed with MX Sheet Version 2 and MX Sheet Version 1.

Install MX Sheet Version 3 after uninstalling MX Sheet Version 2 and MX Sheet Version 1.

■ Utilizing Excel books

Excel books created in MX Sheet Version 2 and MX Sheet Version 1 can be used in MX Sheet Version 2 without modifications.

Precautions

- The operation of the following case is not supported: when opening an Excel book saved in Excel (32-bit version) in Excel (64-bit version) or opening an Excel book saved in Excel(64-bit version) in Excel (32-bit version).
- If the cell area is set with more than 65536 rows, use MX Sheet Version 3.004E or later.

REVISIONS

*The manual number is given on the bottom left of the back cover.

Revision date	*Manual number	Description
April 2021	SH(NA)-082390ENG-A	First edition
November 2021	SH(NA)-082390ENG-B	■Added or modified parts Section 1.1, Section 1.4, Section 3.2, Section 4.2, Chapter 11, Section 12.1, Appendix 1
March 2022	SH(NA)-082390ENG-C	■Added or modified parts Section 1.1, Section 1.3, Section 1.4, Chapter 2, Chapter 3, Chapter 4, Chapter 5, Chapter 6, Chapter 7, Chapter 8, Chapter 9, Chapter 10, Chapter 11, Chapter 12, Chapter 13, Chapter 14, Appendix 1, Appendix 9, Appendix 10, Appendix 11
October 2022	SH(NA)-082390ENG-D	■Added or modified parts GENERIC TERMS AND ABBREVIATIONS, Section 1.1, Section 1.3, Chapter 2, Section 3.2, Section 7.1, Section 11.1, Section 11.3, Chapter 13, Appendix 1, Appendix 9, Appendix 11
May 2023	SH(NA)-082390ENG-E	■Added or modified parts Section 1.1, Section 1.3, Section 3.2, Appendix 1, Appendix 11
October 2023	SH(NA)-082390ENG-F	■Added or modified parts Section 1.1, Section 1.4, Appendix 9
April 2024	SH(NA)-082390ENG-G	■Added or modified parts Section 1.4, Section 3.2, Section 3.3, Section 3.4, Section 3.5, Section 3.6, Appendix 1

Japanese manual number: SH-082389-G

This manual confers no industrial property rights or any rights of any other kind, nor does it confer any patent licenses. Mitsubishi Electric Corporation cannot be held responsible for any problems involving industrial property rights which may occur as a result of using the contents noted in this manual.

© 2021 MITSUBISHI ELECTRIC CORPORATION

INFORMATION AND SERVICES

For further information and services, please contact your local Mitsubishi Electric sales office or representative.
Visit our website to find our locations worldwide.

MITSUBISHI ELECTRIC Factory Automation Global Website
Locations Worldwide
www.MitsubishiElectric.com/fa/about-us/overseas/

TRADEMARKS

Intel is either a registered trademark or a trademark of Intel Corporation in the United States and/or other countries.

Microsoft, Excel, Visual Basic, Visual C++, Visual C#, Visual Studio, and Windows are trademarks of the Microsoft group of companies.

The company names, system names and product names mentioned in this manual are either registered trademarks or trademarks of their respective companies.

In some cases, trademark symbols such as [™] or [®] are not specified in this manual.

COPYRIGHTS

The screens (screenshots) are used in accordance with the Microsoft Corporation guideline.

SH(NA)-082390ENG-G(2404)

MODEL: MXSV3-O-E

MITSUBISHI ELECTRIC CORPORATION

HEAD OFFICE: TOKYO BLDG., 2-7-3, MARUNOUCHI, CHIYODA-KU, TOKYO 100-8310, JAPAN
NAGOYA WORKS: 1-14, YADA-MINAMI 5-CHOME, HIGASHI-KU, NAGOYA 461-8670, JAPAN

When exported from Japan, this manual does not require application to the
Ministry of Economy, Trade and Industry for service transaction permission.

Specifications subject to change without notice.